



Monticello Nuclear Generating Plant
2807 W County Road 75
Monticello, MN 55362

May 10, 2012

L-MT-12-042
Technical Specification 5.6.1

U.S. Nuclear Regulatory Commission
ATTN: Document Control Desk
Washington, DC 20555-0001

Monticello Nuclear Generating Plant
Docket 50-263
Renewed Facility Operating License No. DPR-22

2011 Annual Radiological Environmental Operating Report

In accordance with the Monticello Nuclear Generating Plant Technical Specification 5.6.1, the Northern States Power Company, a Minnesota corporation (NSPM), doing business as Xcel Energy, is submitting the Annual Radiological Environmental Operating Report for the year 2011.

Summary of Commitments

This letter makes no new commitments and no revisions to existing commitments.



Timothy J. O'Connor
Site Vice President, Monticello Nuclear Generating Plant
Northern States Power Company - Minnesota

Enclosure

cc: Administrator, Region III, USNRC
Project Manager, Monticello, USNRC
Resident Inspector, Monticello, USNRC
Minnesota Department of Commerce

JEAS
MRR

ENCLOSURE 1

**RADIOLOGICAL ENVIRONMENTAL OPERATING REPORT
JANUARY 1 – DECEMBER 31, 2011**

68 pages follow



XCEL ENERGY CORPORATION

MONTICELLO NUCLEAR GENERATING PLANT
DOCKET NO. 50-263 LICENSE NO. DPR-22

ANNUAL REPORT
TO THE
UNITED STATES NUCLEAR REGULATORY COMMISSION

Radiological Environmental Monitoring Program

January 1 to December 31, 2011

Prepared under Contract by

ENVIRONMENTAL, Inc.
Midwest Laboratory

Project No. 8010

Approved:

A handwritten signature in black ink, appearing to read 'B. Grob', is written over a horizontal line.

Bronia Grob, M.S.
Laboratory Manager

PREFACE

The staff of Environmental, Inc., Midwest Laboratory was responsible for the acquisition of data presented in this report. Samples were collected by personnel of the Monticello Nuclear Generating Plant, operated by Northern States Power Co. -Minnesota for XCEL Energy Corporation. This report was prepared by Environmental, Inc., Midwest Laboratory.

TABLE OF CONTENTS

<u>No.</u>		<u>Page</u>
	Preface	ii
	List of Tables	iv
	List of Figures	v
1.0	INTRODUCTION	1
2.0	SUMMARY	2
3.0	RADIOLOGICAL ENVIRONMENTAL MONITORING PROGRAM (REMP)	3
	3.1 Program Design and Data Interpretation	3
	3.2 Program Description	4
	3.3 Program Execution	5
	3.4 Laboratory Procedures	6
	3.5 Program Modifications	6
	3.6 Land Use Census	6
4.0	RESULTS AND DISCUSSION	7
	4.1 Atmospheric Nuclear Detonations and Nuclear Accidents	7
	4.2 Summary of Preoperational Data	7
	4.3 Program Findings	8
5.0	FIGURES AND TABLES	12
6.0	REFERENCES	24

APPENDICES

A	Interlaboratory Comparison Program Results	A-1
B	Data Reporting Conventions	B-1
C	Maximum Permissible Concentrations of Radioactivity in Air and Water Above Natural Background in Unrestricted Area	C-1
D	Sampling Location Maps	D-1
E	Ground Water Monitoring Well Samples	E-1

LIST OF TABLES

<u>No.</u>	<u>Title</u>	<u>Page</u>
5.1	Sample Collection and Analysis Program	13
5.2	Sampling Locations	14
5.3	Missed Collections and Analyses	17
5.4	Radiation Environmental Monitoring Program Summary	20

The following tables are in the Appendices:

Appendix A

A-1	Interlaboratory Comparison Program Results	A1-1
A-2	Thermoluminescent dosimeters (TLDs)	A2-1
A-3	In-house Spiked Samples	A3-1
A-4	In-house "Blank" Samples	A4-1
A-5	In-house "Duplicate" Samples	A5-1
A-6	Department of Energy MAPEP comparison results	A6-1
A-7	Environmental Resources Associates, Crosscheck Program Results (EML study replacement)	A7-1
	Attachment A: Acceptance criteria for spiked samples	A2

Appendix C

C-1	Maximum Permissible Concentrations of Radioactivity in air and water above background in unrestricted areas	C-2
-----	--	-----

Appendix E

E-1	Sample Collection and Analysis Program, Ground Water,	E-6
E-2	Sampling Locations for Ground Water Monitoring Wells	E-6
E-3	Ground Water Monitoring Program Summary	E-7

LIST OF FIGURES

<u>No.</u>	<u>Title</u>	<u>Page</u>
5-1	Offsite Ambient Radiation (TLDs), inner versus outer ring locations.....	18
5-2	Airborne Particulates; analysis for gross beta, average-mean of all indicator locations versus control location	19

The following figures are located in the Appendices:

Appendix D

D-1	Sample collection and analysis program: TLD locations, Inner Ring	D-2
D-2	Sample collection and analysis program: TLD locations, Outer Ring	D-3
D-3	Sample collection and analysis program: TLD locations, Controls	D-4
D-4	Sample collection and analysis program: Radiation Environmental Monitoring Program, Milk sampling locations	D-5
D-5	Sample collection and analysis program: Radiation Environmental Monitoring Program, Sludge, Ground water and Shoreline sampling locations.....	D-6

Appendix E

E-1	Sample collection and analysis program: Ground water, On-site monitoring well locations.....	E-8
-----	--	-----

1.0 INTRODUCTION

This report summarizes and interprets results of the Radiological Environmental Monitoring Program (REMP) conducted by Environmental, Inc., Midwest Laboratory for the Monticello Nuclear Generating Plant, Monticello, Minnesota, during the period January - December, 2011. This Program monitors the levels of radioactivity in the air, terrestrial, and aquatic environments in order to assess the impact of the Plant on its surroundings.

Tabulations of the individual analyses made during the year are not included in this report. These data are included in a reference document (Environmental, Inc., Midwest Laboratory, 2011a) available at the Monticello Nuclear Generating Plant, Chemistry and Radiation Protection Department.

The Monticello Nuclear Generating Plant is a boiling water reactor with a nominal generating capacity of 600 MWe. It is located on the Mississippi River in Wright County, Minnesota, owned by Xcel Energy Corporation and operated by Northern States Power Co.-Minnesota. Initial criticality was achieved on December 10, 1970. Full power was achieved March 5, 1971 and commercial operation began on June 30, 1971.

2.0 SUMMARY

The Radiological Environmental Monitoring Program (REMP) required by the U.S. Nuclear Regulatory Commission (NRC) Technical Specifications and the Offsite Dose Calculation Manual (ODCM) for the Monticello Nuclear Generating Plant is described. Results for the year 2011 are summarized and discussed.

Program findings show background levels of radioactivity in the environmental samples collected in the vicinity of the Monticello Nuclear Generating Plant, with the exception of the period from March 17 through May 11, 2011. The detection of iodine-131 in charcoal cartridges and milk and slight elevations of Cs-134 and Cs-137 in air particulate composites are consistent with and attributable to radioactive elements released from the Fukushima Daiichi reactors or fuel pools in the aftermath of the March 11, 2011 Japanese earthquake and tsunami.

3.0 RADIOLOGICAL ENVIRONMENTAL MONITORING PROGRAM (REMP)

3.1 Program Design and Data Interpretation

The purpose of the Radiological Environmental Monitoring Program (REMP) at the Monticello Nuclear Generating Plant is to assess the impact of the Plant on its environment. For this purpose, samples are collected from the air, terrestrial, and aquatic environments and analyzed for radioactive content. In addition, ambient gamma radiation levels are monitored by thermoluminescent dosimeters (TLD's).

Sources of environmental radiation include the following:

- (1) Natural background radiation arising from cosmic rays and primordial radionuclides;
- (2) Fallout from atmospheric nuclear detonations;
- (3) Releases from nuclear power plants;
- (4) Industrial and medical radioactive waste; and
- (5) Fallout from nuclear accidents.

In interpreting the data, effects due to the Plant must be distinguished from those due to other sources.

A major interpretive aid in assessment of these effects is the design of the monitoring program at the Monticello Plant which is based on the indicator-control concept. Most types of samples are collected both at indicator locations (nearby, downwind, or downstream) and at control locations (distant, upwind, or upstream). A plant effect would be indicated if the radiation level at an indicator location was significantly larger than that at the control location. The difference would have to be greater than could be accounted for by typical fluctuations in radiation levels arising from other sources.

An additional interpretive technique involves analyses for specific radionuclides present in environmental samples collected from the Plant site. The Plant's monitoring program includes analyses for tritium and iodine-131. Most samples are also analyzed for gamma-emitting isotopes with results for the following groups quantified: zirconium-95, cesium-137, cerium-144, beryllium-7, and potassium-40. The first three gamma-emitting isotopes were selected as radiological impact indicators because of the different characteristic proportions in which they appear in the fission product mix produced by a nuclear reactor and that produced by a nuclear detonation. Each of the three isotopes is produced in roughly equivalent amounts by a reactor: each constitutes about 10% of the total activity of fission products 10 days after reactor shutdown. On the other hand, 10 days after a nuclear explosion, the contributions of zirconium-95, cerium-144, and cesium-137 to the activity of the resulting debris are in the approximate ratio 4:1:0.03 (Eisenbud, 1963). Beryllium-7 is of cosmogenic origin and potassium-40 is a naturally-occurring isotope. They were chosen as calibration monitors and should not be considered as radiological impact indicators. The other group quantified consists of niobium-95, ruthenium-103 and -106, cesium-134, barium-lanthanum-140, and cerium-141. These isotopes are released in small quantities by nuclear power plants, but to date their major source of injection into the general environment has been atmospheric nuclear testing. Nuclides of the final group, manganese-54, iron-59, cobalt-58 and -60, and zinc-65, are activation products and arise from activation of corrosion products. They are typical components of a nuclear power plant's effluents, but are not produced in significant quantities by nuclear detonations.

Other means of distinguishing sources of environmental radiation are employed in interpreting the data. Current radiation levels are compared with previous levels, including those measured before the plant became operational. Results of the Plant's Monitoring Program can be related to those obtained in other parts of the world. Finally, results can be related to events known to cause elevated levels of radiation in the environment, e.g., atmospheric nuclear detonations.

3.2 Program Description

The sampling and analysis schedule for the Radiological Environmental Monitoring Program (REMP) at the Monticello Plant is summarized in Table 5.1 and briefly reviewed below. Table 5.2 defines the sampling location codes used in Table 5.1 and specifies for each location its type (indicator or control) and its distance, direction, and sector relative to the plant site. To assure that sampling is carried out in a reproducible manner, detailed sampling procedures have been prescribed (Monticello Generating Plant REMP Surveillances, Current Revision). Maps of sampling locations are included in Appendix D.

To monitor the air environment, airborne particulates are collected on membrane filters by continuous pumping at five locations. Also, airborne iodine is collected by continuous pumping through charcoal filters at all of these locations. Filters are changed and counted weekly. Particulate filters are analyzed for gross beta activity and charcoal filters for iodine-131. Quarterly composites of particulate filters from each location are determined by gamma spectroscopy. One of the five locations is a control (M-1), and four are indicators (M-2, M-3, M-4, M-5). One of the indicators is located in the geographical sector expected to be most susceptible to any atmospheric emissions from the Plant (highest D/Q sector).

Ambient gamma radiation is monitored at forty locations, using $\text{CaSO}_4:\text{Dy}$ dosimeters with four sensitive areas at each location: fourteen in an inner ring in the general area of the site boundary, sixteen in the outer ring within 4-5 mile radius, six at special interest locations and four control locations, outside a 10 mile radius from the plant. They are replaced and measured quarterly.

Milk sampling from two goat farms (one indicator and one control), was added to the program in the fourth quarter of 2010. Samples are collected monthly from November through April and biweekly during the growing season (May - October), when animals may be on pasture. The samples are analyzed for iodine-131 and gamma-emitting isotopes. In addition, pasture grass and vegetation are collected from locations M-41, M-42 and M-43 (C) and analyzed for iodine-131 and other gamma emitting isotopes, as substitute for dairy sampling.

Vegetables, corn and potatoes are collected annually if fields are irrigated by water in which liquid radioactive effluent has been discharged. Analysis is done for gamma-emitting isotopes.

Ground water is monitored by quarterly collections from three off-site locations (one control and two indicators) and one on-site Plant well. To prevent possible groundwater contamination due to plant operations, samples from seventeen on-site monitoring wells are collected and analyzed for tritium and gamma emitting isotopes. The Ground Water Monitoring Program is further described in Appendix E.

Quarterly collections of storm water runoff were added to monitor another possible pathway to the groundwater aquifer. The samples are analyzed for tritium and gamma emitting isotopes (Appendix E).

River water is collected weekly at two locations, one upstream of the plant and one downstream. Monthly composites are analyzed for gamma-emitting isotopes. Quarterly composites are analyzed for tritium.

Drinking water is collected weekly from the City of Minneapolis water supply, which is taken from the Mississippi River downstream of the Plant. Monthly composites are analyzed for gross beta, iodine-131, and gamma-emitting isotopes. Quarterly composites are analyzed for tritium.

The aquatic environment is also monitored by semi-annual upstream and downstream collections of fish, invertebrates, and shoreline sediments. Shoreline sediment is also collected from one downstream recreational location. All samples are analyzed for gamma-emitting isotopes.

3.3 Program Execution

The Program was executed as described in the preceding section with the following exceptions:

(1) Air Particulates / Air Iodine:

No air particulate / air iodine sample was available from location M-01 for the week ending June 29, 2011. There was no power, due to an open fuse.

No air particulate/air iodine sample was available from location M-03 for the week ending September 14, 2011. Run-time was significantly lower than expected.

(2) Thermoluminescent Dosimeters:

The TLD for location M-05S was missing in the field for the third quarter, 2011.
The TLD for location M-1B was missing in the field for the fourth quarter, 2011.

(3) Surface Water:

Surface water was not collected at location M-08 during the months of January and February, 2011, due to unsafe ice conditions. The June 14, 2011 sample for composite was damaged in transit.

(4) Well Water:

Well water was not collected at location MW-1 in January, 2011.
The January, 2011 sample collected from MW-12A sample was damaged in transit.

Well water from location MW-13A, October 17, 2011, was damaged in transit.

(5) Milk

Milk was not available from locations M-16 and M-17 for January and February, 2011 collections. No milk was available from location M-17 after November 9, 2011.

(6) Invertebrates

Bottom organisms were not collected in the Spring of 2011, due to high river levels.
Bottom organisms could not be collected from control location M-8 in the Fall of 2011, due to high river levels.

Deviations from the program are summarized in Table 5.3.

3.4 Laboratory Procedures

The iodine-131 analyses in milk and drinking water were made using a sensitive radiochemical procedure which involves separation of the iodine using an ion-exchange method and solvent extraction and subsequent beta counting.

Gamma-spectroscopic analyses are performed using high-purity germanium (HPGe) detectors. Levels of iodine-131 in cabbage and natural vegetation and concentrations of airborne iodine-131 in charcoal samples were determined by gamma spectroscopy.

3.4 Laboratory Procedures (continued)

Tritium concentrations are determined by liquid scintillation.

Analytical Procedures used by Environmental, Inc. are on file and are available for inspection. Procedures are based on those prescribed by the Health and Safety Laboratory of the U.S. Dep't of Energy, Edition 28, 1997, U.S. Environmental Protection Agency for Measurement of Radioactivity in Drinking Water, 1980, and the U.S. Environmental Protection Agency, EERF, Radiochemical Procedures Manual, 1984.

Environmental, Inc., Midwest Laboratory has a comprehensive quality control/quality assurance program designed to assure the reliability of data obtained. Details of the QA Program are presented elsewhere (Environmental, Inc., Midwest Laboratory, 2011). The QA Program includes participation in Interlaboratory Comparison (crosscheck) Programs. Results obtained in the crosscheck programs are presented in Appendix A.

3.5 Program Modifications

There were no program modifications made for 2011.

3.6 Land Use Census

In accordance with the MNGP Chemistry Manual, Procedure I.05.41, "Annual Land Use Census and Critical Receptor Identification", a land use census shall be conducted and shall identify the location of the nearest milk animal, the nearest residence, and the nearest garden of greater than 500 ft² producing fresh leafy vegetables, in each of the 16 meteorological sectors within a distance of 5 miles. The census shall also identify the locations of all milk animals and all 500 ft² or greater gardens producing broad leaf vegetation in each of the meteorological sectors within a distance of three miles. This census shall be conducted at least once per year between the dates of May 1 and October 31. New locations shall be added to the radiation environmental monitoring program within 30 days and sampling locations having lower calculated doses or a lower dose commitment may be deleted from this monitoring program after October 31 of the year in which the land use census was conducted.

The 2011 land use census was conducted between August 30 and September 7, 2011.

In the WNW and NW sectors, the highest D/Q value for nearest garden increased by greater than 20%. Closer gardens were identified. The highest D/Q locations for nearest resident and milk animal did not change from the 2010 census. No changes to the sampling procedures were required.

The location for critical receptor did not change from the 2010 census.

Details of the land use census are contained in the Land Use Census and Critical Receptor Report, Monticello Nuclear Generating Plant, Chemistry and Radiation Protection Department.

4.0 RESULTS AND DISCUSSION

All of the scheduled collections and analyses were made except those listed in Table 5.3.

All results are summarized in Table 5.4 in a format recommended by the Nuclear Regulatory Commission in Regulatory Guide 4.8. For each type of analysis of each sampled medium, this table lists the mean and range for all indicator locations and for all control locations. The locations with the highest mean and range are also shown.

4.1 Atmospheric Nuclear Detonations and Nuclear Accidents

The Fukushima Daiichi nuclear accident occurred on March 11, 2011, releasing large amounts of radioactive isotopes into the atmosphere and Pacific Ocean. Positive iodine-131, cesium-134 and cesium-137 activities were detected in environmental background samples from March through May. The accident, rated seven on the International Nuclear Event Scale (INES) compares with Chernobyl, rated level seven, and Three Mile Island rated level five.

There were no atmospheric nuclear tests conducted in the year 2011

4.2 Summary of Preoperational Data

The following constitutes a summary of preoperational studies conducted at the Monticello Nuclear Generating Plant during the years 1968 to 1970, to determine background levels expected in the environment, and provided, where applicable, as a means for comparison with present day levels. Strict comparisons, however, are difficult to make, since background levels of radiation were much higher in these years due to radioactive fallout from the atmosphere. Gross beta measurements in fallout averaged 20,600 pCi/m² in 1969 and 12,000 pCi/m² in 1970. These levels are reflected throughout the various media tested.

In the air environment, ambient gamma radiation (TLDs) averaged 9.1 mRem/4 weeks during preoperational studies (1970). Gross beta in air particulates in 1969 and 1970 averaged 0.20 pCi/m³. Present day levels have stabilized at around 0.025 pCi/m³. Airborne radioiodine remained below detection levels.

In the terrestrial environment of 1968 to 1970, milk, agricultural crops, and soil were monitored. In milk samples, low levels of Cs-137 and Sr-90 were detected. Cs-137 levels averaged 16.7 pCi/L. Soybean crop measurements in 1969 averaged 35.5 pCi/g for gross beta and 0.3 pCi/g for Cs-137. Gross beta measured in soil averaged 51.7 pCi/g. Present day measurements for cesium-137 are below detection levels in milk and agricultural crops.

The aqueous environment was monitored by testing of river water, bottom sediments, fish, aquatic vegetation, and periphyton. Specific location comparison of drinking, river, and well water concentrations for tritium and gross beta are not possible. However, tritium background levels, measured at seven separate locations from 1968 to 1970, averaged 970 pCi/L. Present day environmental samples measure below detection levels. Values for gross beta, measured from 1968 to 1970, averaged 9.8 pCi/L in upstream and downstream Mississippi River water, 4.4 pCi/L for well waters, and 18.6 pCi/L for lake waters. Gamma emitters were below the lower limit of detection (LLD). In shoreline sediments, gross beta background levels in 1970 averaged 49.8 pCi/g for both upstream and downstream samples. Cs-137 activity averaged 0.10 pCi/g for both upstream and downstream samples. Low levels of Cs-137, occasionally observed today can still be attributed to residual activity from atmospheric fallout. Gross beta levels in fish flesh averaged 5.3 pCi/g in 1968 and 1969. Cs-137, measured in 1969 and 1970, averaged 0.044 pCi/g. Gross beta background levels, in 1970, for aquatic vegetation, algae, and periphyton samples measured 86.7 pCi/g, 76.5 pCi/g, and 28.1 pCi/g respectively.

4.3 Program Findings

Results obtained show background levels of radioactivity in environmental samples collected outside of the Site Protected Area in 2011. The trace levels of strontium-90 and cesium-137, still measurable in soil and sediment samples, are generally attributed to deposition of fallout from previous decades.

Tritium was identified in some groundwater samples collected within the site Protected Area.

Ambient Radiation (TLD's)

Ambient radiation was measured in the general area of the site boundary, at an outer ring 4 - 5 mi. distant from the Plant, at special interest areas and at four control locations. The means were similar for both inner and outer rings (14.8 and 14.3 mRem/91 days, respectively). The mean for special interest locations was 14.1 mRem/91 days and the mean for the control locations was 15.5 mRem/91 days. Dose rates measured at the inner and outer ring locations were similar to those observed from 1996 through 2010 and are tabulated below. No plant effect on ambient gamma radiation is indicated (Figure 5-1).

<u>Year</u>	<u>Inner Ring</u>	<u>Outer Ring</u>
<u>Dose rate (mRem/91 days)</u>		
1996	14.0	13.5
1997	13.3	12.8
1998	15.0	14.4
1999	15.1	14.3
2000	15.1	14.5
2001	14.3	13.7
2002	15.9	14.8
2003	15.6	15.0
2004	16.0	15.4
2005	15.6	15.2
2006	16.5	15.6
2007	16.1	15.1
2008	15.2	14.6
2009	14.9	14.4
2010	14.7	14.3
2011	14.8	14.3

Ambient gamma radiation as measured by thermoluminescent dosimetry.
Average quarterly dose rates, Inner vs. Outer Ring locations

Airborne Particulates

The average annual gross beta concentrations in airborne particulates were identical at both indicator and control locations (0.026 pCi/m³), similar to levels observed from 1996 through 2010. The results are tabulated below.

<u>Year</u>	<u>Indicators</u>	<u>Control</u>
<u>Concentration (pCi/m³)</u>		
1996	0.023	0.023
1997	0.023	0.023
1998	0.023	0.023
1999	0.023	0.025
2000	0.027	0.026
2001	0.027	0.026
2002	0.028	0.028
2003	0.027	0.027
2004	0.024	0.024
2005	0.025	0.025
2006	0.024	0.025
2007	0.027	0.028
2008	0.028	0.029
2009	0.029	0.030
2010	0.026	0.026
2011	0.029	0.027

Average annual gross beta concentrations in airborne particulates.

Typically, the highest average readings occur during the months of January and December, and the first and fourth quarters, as observed in 1996 through 2011.

Gamma spectroscopic analysis of quarterly composites of air particulate filters yielded similar results for indicator and control locations. Beryllium-7, which is produced continuously in the upper atmosphere by cosmic radiation (Arnold and Al-Salih, 1955) was detected in all samples; with an average activity of 0.066 pCi/m³ for all locations. In the second quarter, 2011, traces of Cs-134 and Cs-137 were detected in air particulates composited from location M-03. Low levels of radiocesium were observed in air particulates throughout the U.S., following the Fukushima event. All other gamma-emitting isotopes were below their respective LLD limits.

Airborne Iodine

Following the Fukushima Daiichi accident, measurable radioiodine was detected in weekly collections of activated charcoal cartridges. For the weeks ending March 23, March 30 and April 6, 2011, activity for all locations averaged 0.076, 0.056 and 0.109 pCi/m³, respectively. Iodine could still be detected at two locations, M-1 and M-2 for the week ending April 13, 2011 at an average activity of 0.034 pCi/m³. Measurements for the rest of the year were below the required lower limit of detection of 0.030 pCi/m³.

River Water and Drinking Water

Tritium activity measured below the LLD of 500 pCi/L in all samples. Gross beta activity in Minneapolis drinking water averaged 2.2 pCi/L and was similar to average levels observed from 1995 through 2010. Gross beta averages are tabulated below.

Year	Gross Beta (pCi/L)		Year	Gross Beta (pCi/L)
1996	2.1		2004	2.7
1997	2.3		2005	2.8
1998	2.4		2006	2.1
1999	2.2		2007	2.8
2000	2.5		2008	2.1
2001	2.5		2009	2.3
2002	2.9		2010	2.9
2003	3.0		2011	2.2

Average annual concentrations; Gross beta in drinking water.

Comparisons with data reported by the USEPA for Minneapolis drinking water samples collected from 1980 through 2005 indicate that concentrations of these nuclides are remaining fairly constant. Gamma-emitting isotopes were below detection limits in all surface water samples. There was no indication of a plant effect.

Goat Milk

Iodine-131 was detected in milk sampled from locations M-16 and M-17 for the March 30, 2011 collection, at a concentration of 1.5 pCi/L. The activity was also detected in the April and May collections from location M-16 (1.3 and 1.1 pCi/L, respectively). The activity is consistent with releases from Fukushima. All other results were below a detection limit of 0.5 pCi/L in all samples. Cs-137 results were below the LLD level of 5 pCi/L in all samples. No other gamma-emitting isotopes, except naturally-occurring potassium-40, were detected in any milk samples.

In summary, the data for 2011 showed no radiological effects of the plant operation.

Pasture Grass

Pasture grass was collected in August and September, 2011. I-131 concentrations measured below 0.021 pCi/g wet weight in all samples. With the exceptions of naturally-occurring beryllium-7 and potassium-40, no other gamma-emitting isotopes were detected.

Crops

Vegetation collection was not required for 2011. No crops within five miles of the plant, were found using irrigation water from the Mississippi River.

Fish

Fish were collected in May and October. Flesh was separated from the bones and analyzed by gamma spectroscopy. Only naturally-occurring potassium-40 was found in the upstream and downstream samples (3.12 and 2.92 pCi/g wet weight, respectively). Other gamma-emitting isotopes remained below detection limits. There was no indication of a plant effect.

Invertebrates

One sample from downstream location M-09 was obtained in September, 2011. High water prevented further collections. The sample was analyzed by gamma spectroscopy. All gamma-emitting isotopes were below detection limits. There was no indication of any plant effect.

Shoreline Sediments

Upstream, downstream and downstream recreational area shoreline sediment collections were made in July and October of 2011 and analyzed for gamma-emitting isotopes. Low levels of cesium-137 were detected in three of four downstream samples, averaging 0.047 pCi/g dry weight. Similar levels of activity and distribution have been observed since 1978, and are indicative of the influence of fallout deposition. Naturally-occurring potassium-40 was also detected. There was no indication of a plant effect.

Ground Water Monitoring Program

Monitoring Wells (on-site)

Measurable tritium above 500 pCi/L was detected in 13 of 166 samples collected from seventeen on-site monitoring wells. The activities ranged from 540 to 2,317 pCi/L, similar or lower than concentrations seen in 2010. The highest activities were observed at well MW-9A.

Gamma isotopic measurements were below detection limits.

Stormwater Run-off (on-site)

Tritium activity was detected in two of the seven stormwater runoff samples submitted for analysis in 2011 and measured 772 and 585 pCi/L. Gamma isotopic results were below detection limits.

5.0 FIGURES AND TABLES

Table 5.1. Sample collection and analysis program, Monticello Nuclear Generating Plant.

Medium	No.	Location Codes (and Type) ^a	Collection Type and Frequency ^b	Analysis Type and Frequency ^c
Ambient radiation (TLDs)	40	M-01A - M-14A, M-01B - M-16B M-01S - M-06S, M-01C - M-04C	C/Q	Ambient gamma
Airborne Particulates	5	M-1(C), M-2, M-3, M-4, M-5	C/W	GB, GS (QC of each location)
Airborne Iodine	5	M-1(C), M-2, M-3, M-4, M-5	C/W	I-131
Milk	2	M-16, M-17 (C)	G/M	I-131, GS
Pasture grass, Vegetation ^d	3	M-41, M-42, M-43(C)	3x/year	GS
Surface water	2	M-8(C), M-9	G/W	GS(MC), H-3(QC)
Drinking water	1	M-14	G/W	GB(MC), I-131(MC) GS (MC), H-3 (QC)
Well water	4	M-10(C), M-11, M-12, M-27, M-43(C)	G/Q	H-3, GS
On-site monitoring wells	17	M-33 to M-40, M-44 to M-52		
Edible cultivated crops ^e -				
Leafy Vegetable	2	M-27, Available Producer (C)	G/A	I-131
Corn	1	M-19	G/A	GS
Potatoes	1	M-21	G/A	GS
Fish (one species, edible portion)	2	M-8(C), M-9	G/SA	GS
Periphyton or invertebrates	2	M-8(C), M-9	G/SA	GS
Shoreline sediment	3	M-8(C), M-9, M-15	G/SA	GS

^a Location codes are defined in Table 5.2. Control stations are indicated by (C). All other stations are indicators.

^b Collection type is coded as follows: C/ = continuous, G/ = grab. Collection frequency is coded as follows:
W= weekly, M = monthly, Q = quarterly, SA = semiannually, A = annually.

^c Analysis type is coded as follows: GB = gross beta, GS = gamma spectroscopy, H-3 = tritium, I-131 = iodine-131.
Analysis frequency is coded as follows: MC = monthly composite, QC = quarterly composite.

^d Pasture grass and vegetation collections added to supplement dairy sampling.

^e Collected only if the plant discharges radioactive effluent into the river, then only from river irrigated fields.

Table 5.2. Sampling locations, Monticello Nuclear Generating Plant.

Code	Type ^a	Collection Site	Sample Type ^b	Distance and Direction from Reactor
M-1	C	Air Station M-1	AP, AI	11.0 mi @ 307°/NW
M-2		Air Station M-2	AP, AI	0.8 mi @ 140°/SE
M-3		Air Station M-3	AP, AI	0.6 mi @ 104°/ESE
M-4		Air Station M-4	AP, AI	0.8 mi @ 147°/SSE
M-5		Air Station M-5	AP, AI	2.6 mi @ 134°/SE
M-8	C	Upstream of Plant Intake	SW, SS, BO, F	< 1000' upstream
M-9		Downstream of Plant Discharge	SW, SS, BO, F	< 1000' downstream
M-10	C	Campbell Farm	WW	10.6 mi @ 357°/N
M-11		City of Monticello	WW	3.3 mi @ 127°/SE
M-12		Plant Well #1	WW	0.26 mi @ 252°/WSW
M-14		City of Minneapolis	DW	37.0 mi @ 132°/SE
M-15		Montissippi Park	SS	1.27 mi @ 114°/ESE
M-16		Kitzman Farm	M	3.0 mi @ 165°/SSE
M-17	C	Greninger Farm	M	7.8 mi @ 250°/WSW
M-19		River Irrigated Corn Field ^c	VE	
M-21		River Irrigated Potato Field ^c	VE	
M-27		Wise residence (Highest D/Q Garden) ^c	VE, WW	0.64 mi @ 207°/SSW
		a. Available Producer ^c	VE	> 10.0 mi.
M-33		Monitoring Well #1	WW	593' @ 299°/WNW
M-34		Monitoring Well #2	WW	749' @ 301°/WNW
M-35		Monitoring Well #3	WW	770' @ 304°/NW
M-36		Monitoring Well #4	WW	0.1 mi @ 25°/NNE
M-37		Monitoring Well #5	WW	0.1 mi @ 253°/WSW
M-38		Monitoring Well #6	WW	229' @ 228°/SW
M-39		Monitoring Well #7	WW	0.2 mi @ 66°/ENE
M-40		Monitoring Well #8	WW	0.3 mi @ 150°/SSE
M-41		Training Center	VE	0.8 mi @ 151°/SSE
M-42		Biology Station Road	VE	0.6 mi @ 134°/SE
M-43	C	Imholte Farm	VE, WW	12.3 mi @ 313°/NW
M-44		Monitoring Well #9	WW	0.1 mi @ 310°/NW
M-45		Monitoring Well #10	WW	0.1 mi @ 292°/WNW
M-46		Monitoring Well #11	WW	0.1 mi @ 283°/WNW
M-47		Monitoring Well #12A	WW	0.1 mi @ 330°/NW
M-48		Monitoring Well #12B	WW	0.1 mi @ 326°/NW
M-49		Monitoring Well #13A	WW	0.12 mi @ 316°/NW
M-50		Monitoring Well #13B	WW	0.12 mi @ 316°/NW
M-51		Monitoring Well #9B	WW	0.1 mi @ 310°/NW
M-52		Monitoring Well #14	WW	0.17 mi @ 306°/NW
		Storm water Runoff		0.1 mi @ 27°/NE

Table 5.2. Sampling locations, Monticello Nuclear Generating Plant.

Code	Type ^a	Collection Site	Sample Type ^b	Distance and Direction from Reactor
General Area of the Site Boundary				
M-01A		Sherburne Ave. So.	TLD	0.75 mi @ 353°/N
M-02A		Sherburne Ave. So.	TLD	0.79 mi @ 23°/NNE
M-03A		Sherburne Ave. So.	TLD	1.29 mi @ 55°/NE
M-04A		Biology Station Road	TLD	0.5 mi @ 86°/E
M-05A		Biology Station Road	TLD	0.48 mi @ 118°/ESE
M-06A		Biology Station Road	TLD	0.54 mi @ 135°/SE
M-07A		County Road 75	TLD	0.5 mi @ 155°/SSE
M-08A		County Road 75	TLD	0.48 mi @ 172°/S
M-09A		County Road 75	TLD	0.38 mi @ 209°/SSW
M-10A		County Road 75	TLD	0.38 mi @ 226°/SW
M-11A		County Road 75	TLD	0.4 mi @ 239°/WSW
M-12A		County Road 75	TLD	0.5 mi @ 262°/W
M-13A		North Boundary Road	TLD	0.89 mi @ 324°/NW
M-14A		North Boundary Road	TLD	0.78 mi @ 334°/NNW
Approximately 4 to 5 miles Distant from the Plant				
M-01B		Sherco #1 Air Station	TLD	4.66 mi @ 02°/N
M-02B		County Road 11	TLD	4.4 mi @ 18°/NNE
M-03B		County Road 73 & 81	TLD	4.3 mi @ 51°/NE
M-04B		County Road 73 (196th St.)	TLD	4.2 mi @ 67°/ENE
M-05B		City of Big Lake	TLD	4.3 mi @ 89°/E
M-06B		County Road 14 and 196th St.	TLD	4.3 mi @ 117°/ESE
M-07B		Monte Industrial Drive	TLD	4.3 mi @ 136°/SE
M-08B		Residence, Hwy 25 & Davidson Ave.	TLD	4.6 mi @ 162°/SSE
M-09B		Weinand Farm	TLD	4.7 mi @ 178°/S
M-10B		Reisewitz Farm, Acacia Ave.	TLD	4.2 mi @ 204°/SSW
M-11B		Vanlith Farm, 97th Ave.	TLD	4.0 mi @ 228°/SW
M-12B		Lake Maria State Park	TLD	4.2 mi @ 254°/WSW
M-13B		Bridgewater Station	TLD	4.1 mi @ 270°/W
M-14B		Anderson Residence, Cty Rd. 111	TLD	4.3 mi @ 289°/WNW
M-15B		Red Oak Wild Bird Farm	TLD	4.3 mi @ 309°/NW
M-16B		Sand Plain Research Farm	TLD	4.4 mi @ 341°/NNW

Table 5.2. Sampling locations, Monticello Nuclear Generating Plant.

Code	Type ^a	Collection Site	Sample Type ^b	Distance and Direction from Reactor
Special Interest Locations				
M-01S		Oowski Fun Market	TLD	0.66 mi @ 242°/WSW
M-02S		Krone Residence	TLD	0.5 mi @ 224°/SW
M-03S		Big Oaks Park	TLD	1.53 mi @ 102°/ESE
M-04S		Pinewood School	TLD	2.3 mi @ 131°/SE
M-05S		Rivercrest Christian Academy	TLD	3.0 mi @ 118°/ESE
M-06S		Monte Public Works	TLD	2.6 mi @ 134°/SE
M-01C	C	Kirchenbauer Farm	TLD	11.5 mi @ 323°/NW
M-02C	C	County Roads 4 and 15	TLD	11.2 mi @ 47°/NE
M-03C	C	County Rd 19 and Jason Ave.	TLD	11.6 mi @ 130°/SE
M-04C	C	Maple Lake Water Tower	TLD	10.3 mi @ 226°/ SW
Protected Area				
ISFSI-1		ISFSI-1 (neutron) and I-01 (gamma)	TLD	NE corner of ISFSI
ISFSI-2		ISFSI-2 (neutron) and I-02 (gamma)	TLD	North side of ISFSI, center
ISFSI-3		ISFSI-3 (neutron) and I-03 (gamma)	TLD	NW corner of ISFSI
ISFSI-4		ISFSI-4 (neutron) and I-04 (gamma)	TLD	West side of ISFSI, middle
ISFSI-5		ISFSI-5 (neutron) and I-05 (gamma)	TLD	West side of ISFSI, at center of array
ISFSI-6		ISFSI-6 (neutron) and I-06 (gamma)	TLD	SW corner of ISFSI
ISFSI-7		ISFSI-7 (neutron) and I-07 (gamma)	TLD	South side of ISFSI, center
ISFSI-8		ISFSI-8 (neutron) and I-08 (gamma)	TLD	SE corner of ISFSI
ISFSI-9		ISFSI-9 (neutron) and I-09 (gamma)	TLD	East side of ISFSI, at center of array
ISFSI-10		ISFSI-10 (neutron) and I-10 (gamma)	TLD	East side of ISFSI, middle
ISFSI-11		ISFSI-11 (neutron) and I-11 (gamma)	TLD	OCA fence south, on exit road
ISFSI-12		ISFSI-12 (neutron) and I-12 (gamma)	TLD	OCA fence middle, on exit road
ISFSI-13		ISFSI-13 (neutron) and I-13 (gamma)	TLD	OCA fence north, on exit road
ISFSI-14		ISFSI-14 (neutron)	TLD	Posted with TLD M12A
ISFSI-15		ISFSI-15 (neutron)	TLD	Posted with TLD M10A
ISFSI-16		ISFSI-16 (neutron)	TLD	Posted with TLD M02S
Neutron Control A	C		TLD	Posted with TLD M03C
Neutron Control B	C		TLD	Posted with TLD M04C
Neutron Control C	C		TLD	Posted with TLD M02C
Neutron Control D	C		TLD	Posted with TLD M01C

^a "C" denotes control location. All other locations are indicators.

^b Sample Codes:

AP	Airborne particulates	F	Fish
AI	Airborne iodine	SW	River Water
BS	Bottom (river) sediments	SS	Shoreline Sediments
BO	Bottom organisms	TLD	Thermoluminescent Dosimeter
DW	Drinking Water	VE	Vegetation / vegetables
		WW	Well Water.

^c Collected only if the plant discharges radioactive effluent into the river, then only from river irrigated fields.

Table 5.3. MISSED COLLECTIONS AND ANALYSES

All required samples were collected and analyzed as scheduled with the following exceptions:					
Sample Type	Analysis	Location	Collection Date or Period	Reason for not conducting REMP as required	Plans for Preventing Recurrence
SW	Gamma	M-08	January	Water frozen.	None Required
SW	Gamma	M-08	February	Water frozen.	None Required
SW	For composite	M-08	6/14/2011	Sample damaged in transit.	None Required
WW	Gamma, H-3	MW-1	1/17/2011	Well not sampled, frozen.	None Required
WW	Gamma, H-3	MW-12A	1/17/2011	Container damaged in transit.	None Required
WW	Gamma, H-3	MW-13A	10/17/2011	Container damaged in transit.	None Required
TLD	Gamma	M-5S	10/3/2011	TLD missing in field.	Replaced, vandalism
TLD	Gamma	M-1B	1/4/2012	TLD missing in field.	Replaced, vandalism
AP/AI	Beta, I-131	M-1	6/29/2011	No power at sampler.	Power restored by utility.
AP/AI	Beta, I-131	M-3	9/14/2011	Elapsed time low.	Replaced with spare, repaired affected pump.
MI	Gamma, I-131	M-16, 17	1/31/2011	Milking discontinued until Spring.	None Required
MI	Gamma, I-131	M-17	12/14/2011	Milking discontinued for the year.	None Required
BO	Gamma	M-8, M-9	Spring	High water prevented sampling.	None Required
BO	Gamma	M-8	Fall	High water prevented sampling.	None Required

Figure 5-1. Offsite Ambient Radiation (TLDs); Inner Ring versus Outer Ring locations.

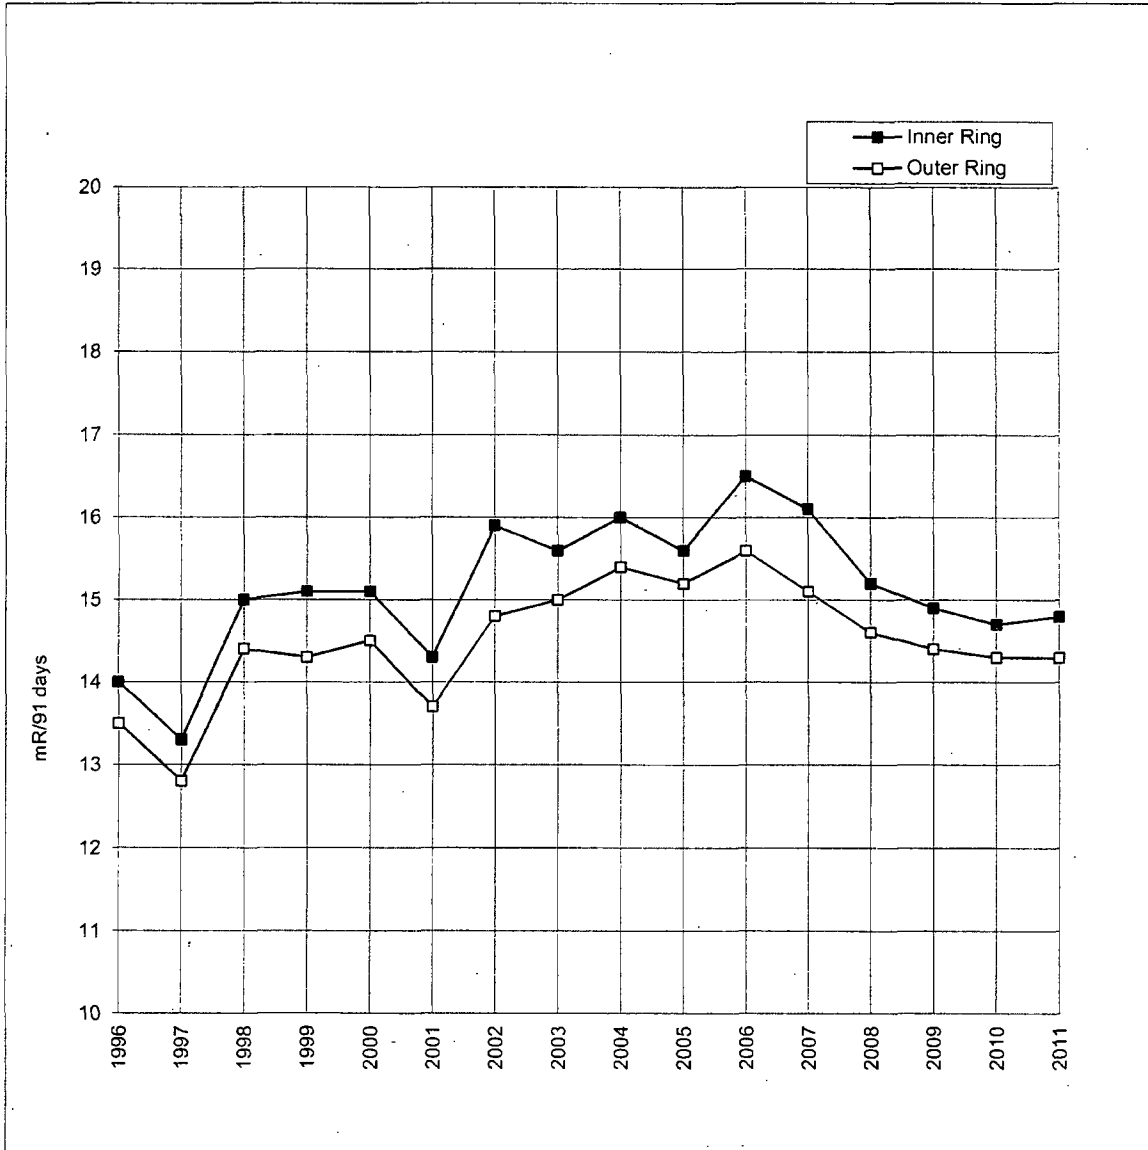


Figure 5-2. Airborne Particulates; analysis for gross beta, average mean of all indicator locations versus control location.

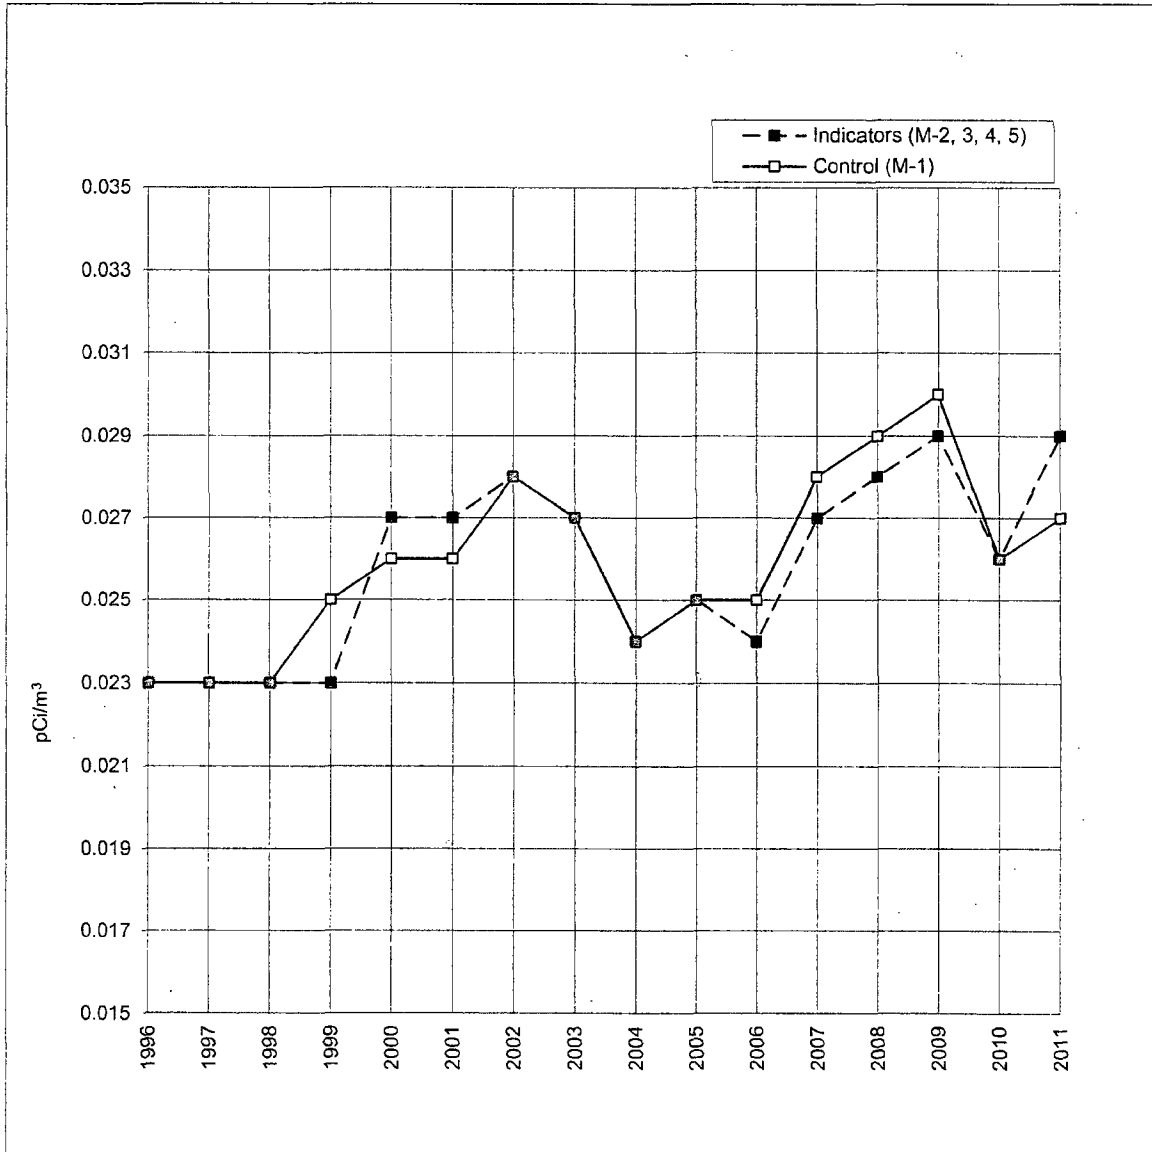


Table 5.4 Radiological Environmental Monitoring Program Summary

Name of Facility	<u>Monticello Nuclear Generating Plant</u>	Docket No.	<u>50-263</u>
Location of Facility	<u>Wright, Minnesota</u>	Reporting Period	<u>January-December, 2011</u>
	(County, State)		

Sample Type (Units)	Type and Number of Analyses ^a	LLD ^b	Indicator Locations Mean (F) ^c Range ^c	Location with Highest Annual Mean		Control Locations Mean (F) ^c Range ^c	Number Non-Routine Results ^e
				Location ^d	Mean (F) ^c Range ^c		
Direct Radiation							
TLD (Inner Ring, General Area at Site Boundary) mRem/91 days)	Gamma 56	3.0	14.8 (56/56) (11.2-18.5)	M-11A, County Rd 75, 0.4 mi @ 250°/WSW	16.3 (4/4) (14.5-18.5)	(See Control below.)	0
TLD (Outer Ring, 4-5 mi. distant) mRem/91 days)	Gamma 63	3.0	14.3 (63/63) (11.0-18.6)	M-07B 4.4 mi @ 135°/SE	15.8 (4/4) (14.8-16.9)	(See Control below.)	0
TLD (Special Interest Areas) mRem/91 days)	Gamma 23	3.0	14.1 (23/23) (9.8-18.6)	M-06S, Mont. Pub. Wks. 2.7 mi @ 136°/SE	17.0 (4/4) (15.6-18.6)	(See Control below.)	0
TLD (Control) mRem/91 days)	Gamma 16	3.0	None	M-03C, Rte. 19 & Jason, 11.6 mi @ 130°/SE	16.5 (4/4) (13.6-18.3)	15.5 (16/16) (12.1-18.3)	0
Airborne Pathway							
Airborne Particulates (pCi/m ³)	GB 258	0.002	0.029 (207/207) (0.010-0.070)	M-4, Air Station 0.8 mi @ 147°/SSE	0.030 (52/52) (0.010-0.070)	0.027 (51/51) (0.007-0.062)	0
	GS 20	0.015	0.067 (16/16) (0.053-0.093)	M-3, Air Station 0.6 mi @ 104°/ESE	0.070 (4/4) (0.061-0.093)	0.065 (4/4) (0.056-0.078)	0
	Mn-54	0.0010	< LLD	-	-	< LLD	0
	Co-58	0.0012	< LLD	-	-	< LLD	0
	Co-60	0.0010	< LLD	-	-	< LLD	0
	Zn-65	0.0018	< LLD	-	-	< LLD	0
	Zr-Nb-95	0.0014	< LLD	-	-	< LLD	0
	Ru-103	0.0013	< LLD	-	-	< LLD	0
	Ru-106	0.0098	< LLD	-	-	< LLD	0
	Cs-134	0.0011	0.0013 (1/16)	M-3, Air Station 0.6 mi @ 104°/ESE	-	< LLD	0
	Cs-137	0.0010	0.0014 (1/16)	M-3, Air Station 0.6 mi @ 104°/ESE	-	< LLD	0
	Ba-La-140	0.0035	< LLD	-	-	< LLD	0
	Ce-141	0.0023	< LLD	-	-	< LLD	0
Ce-144	0.0063	< LLD	-	-	< LLD	0	
Airborne Iodine (pCi/m ³)	I-131 258	0.03	0.077 (13/207) (0.036-0.134)	M-4, Air Station 0.8 mi @ 147°/SSE	0.098 (3/52) (0.061-0.134)	0.067 (4/51) (0.031-0.112)	0

Table 5.4 Radiological Environmental Monitoring Program Summary

Name of Facility Monticello Nuclear Generating Plant Docket No. 50-263
 Location of Facility Wright, Minnesota Reporting Period January-December, 2011
 (County, State)

Sample Type (Units)	Type and Number of Analyses ^a	LLD ^b	Indicator Locations Mean (F) ^c Range ^c	Location with Highest Annual Mean		Control Locations Mean (F) ^c Range ^c	Number Non-Routine Results ^e
				Location ^d	Mean (F) ^c Range ^c		
Waterborne Pathway							
River Water (pCi/L)	H-3 8	500	< LLD	-	-	< LLD	0
	GS 22						
	Mn-54 10		< LLD	-	-	< LLD	0
	Fe-59 30		< LLD	-	-	< LLD	0
	Co-58 10		< LLD	-	-	< LLD	0
	Co-60 10		< LLD	-	-	< LLD	0
	Zn-65 30		< LLD	-	-	< LLD	0
	Zr-Nb-95 15		< LLD	-	-	< LLD	0
	Cs-134 10		< LLD	-	-	< LLD	0
	Cs-137 10		< LLD	-	-	< LLD	0
	Ba-La-140 15		< LLD	-	-	< LLD	0
Ce-144 43		< LLD	-	-	< LLD	0	
Drinking Water (pCi/L)	GB 12	1.0	2.2 (12/12) (1.0-3.0)	M-14, Minneapolis 37.0 mi. @ 132° /SE	2.2 (12/12) (1.0-3.0)	None	0
	I-131 12	1.0	< LLD	-	-	None	0
	H-3 4	500	< LLD	-	-	None	0
	GS 12						
	Mn-54 10		< LLD	-	-	None	0
	Fe-59 30		< LLD	-	-	None	0
	Co-58 10		< LLD	-	-	None	0
	Co-60 10		< LLD	-	-	None	0
	Zn-65 30		< LLD	-	-	None	0
	Zr-Nb-95 15		< LLD	-	-	None	0
	Cs-134 10		< LLD	-	-	None	0
	Cs-137 10		< LLD	-	-	None	0
	Ba-La-140 15		< LLD	-	-	None	0
Ce-144 27		< LLD	-	-	None	0	
Well Water (pCi/L)	H-3 16	500	< LLD	-	-	< LLD	0
	GS 16						
	Mn-54 10		< LLD	-	-	< LLD	0
	Fe-59 30		< LLD	-	-	< LLD	0
	Co-58 10		< LLD	-	-	< LLD	0
	Co-60 10		< LLD	-	-	< LLD	0
	Zn-65 30		< LLD	-	-	< LLD	0
	Zr-Nb-95 15		< LLD	-	-	< LLD	0
	Cs-134 10		< LLD	-	-	< LLD	0
	Cs-137 10		< LLD	-	-	< LLD	0
	Ba-La-140 15		< LLD	-	-	< LLD	0
Ce-144 46		< LLD	-	-	< LLD	0	

Table 5.4 Radiological Environmental Monitoring Program Summary

Name of Facility	<u>Monticello Nuclear Generating Plant</u>	Docket No.	<u>50-263</u>
Location of Facility	<u>Wright, Minnesota</u>	Reporting Period	<u>January-December, 2011</u>
	(County. State)		

Sample Type (Units)	Type and Number of Analyses ^a	LLD ^b	Indicator Locations Mean (F) ^c Range ^c	Location with Highest Annual Mean		Control Locations Mean (F) ^c Range ^c	Number Non-Routine Results ^e
				Location ^d	Mean (F) ^c Range ^c		
Waterborne Pathway							
Invertebrates (pCi/g wet)	GS 1						
	Be-7	0.33	< LLD	-	-	none	0
	K-40	0.65	< LLD	-	-	none	0
	Mn-54	0.024	< LLD	-	-	none	0
	Fe-59	0.075	< LLD	-	-	none	0
	Co-58	0.036	< LLD	-	-	none	0
	Co-60	0.024	< LLD	-	-	none	0
	Zn-65	0.057	< LLD	-	-	none	0
	Zr-Nb-95	0.044	< LLD	-	-	none	0
	Ru-103	0.051	< LLD	-	-	none	0
	Ru-106	0.31	< LLD	-	-	none	0
	Cs-134	0.036	< LLD	-	-	none	0
	Cs-137	0.040	< LLD	-	-	none	0
	Ba-La-140	0.072	< LLD	-	-	none	0
Ce-144	0.12	< LLD	-	-	none	0	
Shoreline Sediments (pCi/g dry)	GS 6						
	Be-7	0.27	< LLD	-	-	< LLD	0
	K-40	0.10	10.30 (4/4) (9.78-11.35)	M-09, Downstream < 1000' of discharge	10.75 (2/2) (10.16-11.35)	10.50 (2/2) (9.51-11.48)	0
	Mn-54	0.022	< LLD	-	-	< LLD	0
	Fe-59	0.068	< LLD	-	-	< LLD	0
	Co-58	0.021	< LLD	-	-	< LLD	0
	Co-60	0.018	< LLD	-	-	< LLD	0
	Zn-65	0.042	< LLD	-	-	< LLD	0
	Nb-95	0.038	< LLD	-	-	< LLD	0
	Zr-95	0.048	< LLD	-	-	< LLD	0
	Ru-103	0.027	< LLD	-	-	< LLD	0
	Ru-106	0.16	< LLD	-	-	< LLD	0
	Cs-134	0.016	< LLD	-	-	< LLD	0
	Cs-137	0.015	0.047 (3/4) (0.028-0.091)	M-09, Downstream < 1000' of discharge	0.065 (2/2) (0.040-0.091)	< LLD	0
Ba-La-140	0.064	< LLD	-	-	< LLD	0	
Ce-144	0.14	< LLD	-	-	< LLD	0	

Table 5.4 Radiological Environmental Monitoring Program Summary

Name of Facility	<u>Monticello Nuclear Generating Plant</u>	Docket No.	<u>50-263</u>
Location of Facility	<u>Wright, Minnesota</u>	Reporting Period	<u>January-December, 2011</u>
	(County, State)		

Sample Type (Units)	Type and Number of Analyses ^a	LLD ^b	Indicator Locations Mean (F) ^c Range ^c	Location with Highest Annual Mean		Control Locations Mean (F) ^c Range ^c	Number Non-Routine Results ^e
				Location ^d	Mean (F) ^c Range ^c		
Ingestion Pathway							
Milk (pCi/L)	I-131 33	0.5	< LLD	-	-	< LLD	0
	GS 33						
	K-40	200	1821 (16/16) (1629-1994)	M-16, Kitzman 3.0 mi @ 165°/SSE	1821 (16 /16) (1629-1994)	1818 (17/17) (1655-1922)	0
	Cs-134	5	< LLD	-	-	< LLD	0
	Cs-137	5	< LLD	-	-	< LLD	0
	Ba-La-140	5	< LLD	-	-	< LLD	0
Vegetation (Pasture Grass, Weeds, Leaves) (pCi/gwet)	GS 9						
	Mn-54	0.011	< LLD	-	-	< LLD	0
	Fe-59	0.027	< LLD	-	-	< LLD	0
	Co-58	0.012	< LLD	-	-	< LLD	0
	Co-60	0.009	< LLD	-	-	< LLD	0
	Zn-65	0.035	< LLD	-	-	< LLD	0
	Nb-95	0.013	< LLD	-	-	< LLD	0
	I-131	0.021	< LLD	-	-	< LLD	0
	Cs-134	0.013	< LLD	-	-	< LLD	0
Cs-137	0.014	< LLD	-	-	< LLD	0	
Fish (pCi/g wet)	GS 10						
	K-40	0.10	3.12 (5/5) (2.55-3.58)	M-09, Downstream < 1000' of discharge	3.12 (5/5) (2.55-3.58)	2.92 (5/5) (2.74-3.21)	0
	Mn-54	0.021	< LLD	-	-	< LLD	0
	Fe-59	0.062	< LLD	-	-	< LLD	0
	Co-58	0.028	< LLD	-	-	< LLD	0
	Co-60	0.025	< LLD	-	-	< LLD	0
	Zn-65	0.033	< LLD	-	-	< LLD	0
	Zr-Nb-95	0.029	< LLD	-	-	< LLD	0
	Cs-134	0.024	< LLD	-	-	< LLD	0
	Cs-137	0.028	< LLD	-	-	< LLD	0
	Ba-La-140	0.067	< LLD	-	-	< LLD	0
Ce-144	0.16	< LLD	-	-	< LLD	0	

^a GB = gross beta, GS = gamma scan.

^b LLD = nominal lower limit of detection based on a 4.66 sigma counting error for background sample.

^c Mean and range are based on detectable measurements only. Fraction of detectable measurements at specified locations is indicated in parentheses (F).

^d Locations are specified: (1) by name, and/or station code and (2) by distance (miles) and direction relative to reactor site.

^e Non-routine results are those which exceed ten times the control station value. If no control station value is available, the result is considered non-routine if it exceeds ten times the typical preoperational value for the medium or location.

6.0 REFERENCES CITED

Arnold, J. R. and H. A. Al-Salih. 1955. Beryllium-7 Produced by Cosmic Rays. Science 121: 451-453.

Eisenbud, M. 1963. Environmental Radioactivity, McGraw-Hill, New York, New York, pp. 213, 275, 276.

Environmental, Inc., Midwest Laboratory.

_____ 2001a through 2012a. Radiation Environmental Monitoring for Monticello Nuclear Generating Plant, Complete Analysis Data Tables, January-December, 2000 through 2011.

_____ 2001b through 2012b. Radiation Environmental Monitoring for Prairie Island Nuclear Generating Plant, Complete Analysis Data Tables, January - December, 2000 through 2011.

_____ 1984a to 2000a. (formerly Teledyne Brown Engineering Environmental Services, Midwest Laboratory) Radiation Environmental Monitoring for Monticello Nuclear Generating Plant, Complete Analysis Data Tables, January - December, 1983 through 1999.

_____ 1984b to 2000b. (formerly Teledyne Brown Engineering Environmental Services, Midwest Laboratory) Radiation Environmental Monitoring for Prairie Island Nuclear Generating Plant, Complete Analysis Data Tables, January - December, 1983 through 1999.

_____ 1979a to 1983a. (formerly Hazleton Environmental Sciences Corporation) Radiation Environmental Monitoring for Monticello Nuclear Generating Plant, Complete Analysis Data Tables, January - December, 1978 through 1982.

_____ 1979b to 1983b. (formerly Hazleton Environmental Sciences Corporation) Radiation Environmental Monitoring for Prairie Island Nuclear Generating Plant, Complete Analysis Data Tables, January - December, 1978 through 1982.

_____ 2009. Quality Assurance Program Manual, Rev. 2, 10 November 2009.

_____ 2009. Quality Control Procedures Manual, Rev. 2, 08 July 2009.

_____ 2009. Quality Control Program, Rev. 2, 12 November 2009.

Gold, S., H.W. Barkhau, B. Shlein, and B. Kahn, 1964. Measurement of Naturally Occurring Radionuclides in Air, in the Natural Environment, University of Chicago Press, Illinois, 369-382.

National Center for Radiological Health, 1968. Radiological Health and Data Reports, Vol. 9, Number 12, 730-746.

Northern States Power Company.

_____ 1969 through 1971. Monticello Nuclear Generating Plant, Environmental Radiation Monitoring Program, Annual Report, June 18, 1968 to December 31, 1968, 1969, 1970. Minneapolis, Minnesota.

_____ 1978 through 2008. Monticello Nuclear Generating Plant, Annual Radiation Environmental Monitoring Report to the U.S. Nuclear Regulatory Commission, January 1, to December 31, 1977 through 2007.

6.0 REFERENCES CITED (continued)

U.S. Dep't of Energy 1997 HASL-300, Edition 28, Procedures Manual, Environmental Measurements Laboratory, New York, NY.

U.S. Environmental Protection Agency .

_____ 1980. Prescribed Procedures for Measurement of Radioactivity in Drinking Water, Cincinnati, Ohio (EPA-600/4-80-032).

_____ 1984. Eastern Environmental Radiation Facility, Radiochemistry Procedures Manual, Montgomery, Alabama (EPA-520/5-84-006).

_____ 2009. RadNet, formerly Environmental Radiation Ambient Monitoring System, Gross Beta in Air, Gross Beta in Drinking Water (MN) 1981– 2005.

Wilson, D. W., G. M. Ward and J. E. Johnson. 1969. In Environmental Contamination by Radioactive Materials, International Atomic Energy Agency. p.125.

Xcel Energy Corporation.

_____ 2009 to 2012. Monticello Nuclear Generating Plant, Annual Radiation Environmental Monitoring Report to the U.S. Nuclear Regulatory Commission, January 1 to December 31, 2008 through 2011. Minneapolis, Minnesota.

_____ 2009 to 2012. Prairie Island Nuclear Generating Plant, Annual Radiation Environmental Monitoring Report to the U.S. Nuclear Regulatory Commission, January 1 to December 31, 2008 through 2011. Minneapolis, Minnesota.



APPENDIX A

INTERLABORATORY COMPARISON PROGRAM RESULTS

NOTE: Environmental Inc., Midwest Laboratory participates in intercomparison studies administered by Environmental Resources Associates, and serves as a replacement for studies conducted previously by the U.S. EPA Environmental Monitoring Systems Laboratory, Las Vegas, Nevada. Results are reported in Appendix A. TLD Intercomparison results, in-house spikes, blanks, duplicates and mixed analyte performance evaluation program results are also reported. Appendix A is updated four times a year; the complete Appendix is included in March, June, September and December monthly progress reports only.

January through December, 2011

Appendix A

Interlaboratory Comparison Program Results

Environmental, Inc., Midwest Laboratory has participated in interlaboratory comparison (crosscheck) programs since the formulation of its quality control program in December 1971. These programs are operated by agencies which supply environmental type samples containing concentrations of radionuclides known to the issuing agency but not to participant laboratories. The purpose of such a program is to provide an independent check on a laboratory's analytical procedures and to alert it of any possible problems.

Participant laboratories measure the concentration of specified radionuclides and report them to the issuing agency. Several months later, the agency reports the known values to the participant laboratories and specifies control limits. Results consistently higher or lower than the known values or outside the control limits indicate a need to check the instruments or procedures used.

Results in Table A-1 were obtained through participation in the environmental sample crosscheck program administered by Environmental Resources Associates, serving as a replacement for studies conducted previously by the U.S. EPA Environmental Monitoring Systems Laboratory, Las Vegas, Nevada.

Table A-2 lists results for thermoluminescent dosimeters (TLDs), via International Intercomparison of Environmental Dosimeters, when available, and internal laboratory testing.

Table A-3 lists results of the analyses on in-house "spiked" samples for the past twelve months. All samples are prepared using NIST traceable sources. Data for previous years available upon request.

Table A-4 lists results of the analyses on in-house "blank" samples for the past twelve months. Data for previous years available upon request.

Table A-5 lists REMP specific analytical results from the in-house "duplicate" program for the past twelve months. Acceptance is based on the difference of the results being less than the sum of the errors. Complete analytical data for duplicate analyses is available upon request.

The results in Table A-6 were obtained through participation in the Mixed Analyte Performance Evaluation Program.

Results in Table A-7 were obtained through participation in the environmental sample crosscheck program administered by Environmental Resources Associates, serving as a replacement for studies conducted previously by the Environmental Measurement Laboratory Quality Assessment Program (EML).

Attachment A lists the laboratory precision at the 1 sigma level for various analyses. The acceptance criteria in Table A-3 is set at ± 2 sigma.

Out-of-limit results are explained directly below the result.

Attachment A

ACCEPTANCE CRITERIA FOR "SPIKED" SAMPLES

LABORATORY PRECISION: ONE STANDARD DEVIATION VALUES FOR VARIOUS ANALYSES^a

Analysis	Level	One standard deviation for single determination
Gamma Emitters	5 to 100 pCi/liter or kg > 100 pCi/liter or kg	5.0 pCi/liter 5% of known value
Strontium-89 ^b	5 to 50 pCi/liter or kg > 50 pCi/liter or kg	5.0 pCi/liter 10% of known value
Strontium-90 ^b	2 to 30 pCi/liter or kg > 30 pCi/liter or kg	5.0 pCi/liter 10% of known value
Potassium-40	≥ 0.1 g/liter or kg	5% of known value
Gross alpha	≤ 20 pCi/liter > 20 pCi/liter	5.0 pCi/liter 25% of known value
Gross beta	≤ 100 pCi/liter > 100 pCi/liter	5.0 pCi/liter 5% of known value
Tritium	≤ 4,000 pCi/liter > 4,000 pCi/liter	± 1σ = 169.85 x (known) ^{0.0933} 10% of known value
Radium-226,-228	≥ 0.1 pCi/liter	15% of known value
Plutonium	≥ 0.1 pCi/liter, gram, or sample	10% of known value
Iodine-131, Iodine-129 ^b	≤ 55 pCi/liter > 55 pCi/liter	6 pCi/liter 10% of known value
Uranium-238, Nickel-63 ^b Technetium-99 ^b	≤ 35 pCi/liter > 35 pCi/liter	6 pCi/liter 15% of known value
Iron-55 ^b	50 to 100 pCi/liter > 100 pCi/liter	10 pCi/liter 10% of known value
Other Analyses ^b	---	20% of known value

^a From EPA publication, "Environmental Radioactivity Laboratory Intercomparison Studies Program, Fiscal Year, 1981-1982. EPA-600/4-81-004.

^b Laboratory limit.

TABLE A-1. Interlaboratory Comparison Crosscheck program, Environmental Resource Associates (ERA)^a.

Lab Code	Date	Analysis	Concentration (pCi/L)			Acceptance
			Laboratory Result ^b	ERA Result ^c	Control Limits	
STW-1243	04/04/11	Sr-89	68.2 ± 5.8	63.2	51.1 - 71.2	Pass
STW-1243	04/04/11	Sr-90	44.3 ± 2.4	42.5	31.3 - 48.8	Pass
STW-1244	04/04/11	Ba-133	69.8 ± 3.9	75.3	63.0 - 82.8	Pass
STW-1244	04/04/11	Co-60	87.9 ± 3.8	88.8	79.9 - 100.0	Pass
STW-1244	04/04/11	Cs-134	69.5 ± 3.7	72.9	59.5 - 80.2	Pass
STW-1244	04/04/11	Cs-137	77.9 ± 5.3	77.0	69.3 - 87.4	Pass
STW-1244	04/04/11	Zn-65	105.2 ± 8.4	98.9	89.0 - 118.0	Pass
STW-1245	04/04/11	Gr. Alpha	41.5 ± 2.3	50.1	26.1 - 62.9	Pass
STW-1245	04/04/11	Gr. Beta	48.9 ± 1.8	49.8	33.8 - 56.9	Pass
STW-1246	04/04/11	I-131	26.6 ± 1.7	27.5	22.9 - 32.3	Pass
STW-1247	04/04/11	Ra-226	13.2 ± 0.6	12.1	9.0 - 14.0	Pass
STW-1247	04/04/11	Ra-228	11.2 ± 0.6	11.6	7.6 - 14.3	Pass
STW-1247	04/04/11	Uranium	36.4 ± 0.6	39.8	32.2 - 44.4	Pass
STW-1248	04/04/11	H-3	10322 ± 285	10200.0	8870 - 11200	Pass
STW-1256	10/07/11	Sr-89	68.7 ± 6.0	69.7	56.9 - 77.9	Pass
STW-1256	10/07/11	Sr-90	36.9 ± 2.4	41.1	30.2 - 47.2	Pass
STW-1257	10/07/11	Ba-133	88.2 ± 7.8	96.9	81.8 - 106.0	Pass
STW-1257	10/07/11	Co-60	116.5 ± 7.1	119.0	107.0 - 133.0	Pass
STW-1257 ^d	10/07/11	Cs-134	38.8 ± 8.0	33.4	26.3 - 36.7	Fail
STW-1257	10/07/11	Cs-137	45.6 ± 7.3	44.3	39.4 - 51.7	Pass
STW-1257	10/07/11	Zn-65	84.9 ± 15.4	76.8	68.9 - 92.5	Pass
STW-1258	10/07/11	Gr. Alpha	35.7 ± 3.8	53.2	27.8 - 66.6	Pass
STW-1258	10/07/11	Gr. Beta	36.1 ± 3.3	45.9	30.9 - 53.1	Pass
STW-1259	10/07/11	I-131	25.0 ± 1.1	27.5	22.9 - 32.3	Pass
STW-1260	10/07/11	Ra-226	12.2 ± 0.6	11.6	8.7 - 13.4	Pass
STW-1260	10/07/11	Ra-228	11.5 ± 1.7	10.3	6.7 - 12.8	Pass
STW-1260	10/07/11	Uranium	46.6 ± 0.5	48.6	39.4 - 54.0	Pass
STW-1261	10/07/11	H-3	17435 ± 382	17400	15200 - 19100	Pass

^a Results obtained by Environmental, Inc., Midwest Laboratory as a participant in the crosscheck program for proficiency testing in drinking water conducted by Environmental Resources Associates (ERA).

^b Unless otherwise indicated, the laboratory result is given as the mean ± standard deviation for three determinations.

^c Results are presented as the known values, expected laboratory precision (1 sigma, 1 determination) and control limits as provided by ERA.

^d The sample was reanalyzed. Result of reanalysis was acceptable, 32.9 ± 7.4 pCi/L.

TABLE A-2. Thermoluminescent Dosimetry, (TLD, CaSO₄: Dy Cards).

Lab Code	Date	Description	mR			Acceptance
			Known Value	Lab Result ± 2 sigma	Control Limits	
<u>Environmental, Inc.</u>						
2010-2	12/13/2010	100 cm.	4.94	4.65 ± 0.57	3.46 - 6.42	Pass
2010-2	12/13/2010	110 cm.	4.09	3.50 ± 0.74	2.86 - 5.32	Pass
2010-2	12/13/2010	120 cm.	3.43	2.68 ± 0.36	2.40 - 4.46	Pass
2010-2	12/13/2010	150 cm.	2.2	1.75 ± 0.42	1.54 - 2.86	Pass
2010-2	12/13/2010	180 cm.	1.53	1.32 ± 0.52	1.07 - 1.99	Pass
2010-2	12/13/2010	40 cm.	30.89	38.56 ± 2.11	21.62 - 40.16	Pass
2010-2	12/13/2010	50 cm.	19.77	23.35 ± 1.82	13.84 - 25.70	Pass
2010-2	12/13/2010	60 cm.	13.73	14.53 ± 1.24	9.61 - 17.85	Pass
2010-2	12/13/2010	60 cm.	13.73	15.84 ± 1.53	9.61 - 17.85	Pass
2010-2	12/13/2010	80 cm.	7.72	8.33 ± 0.74	5.40 - 10.04	Pass
2010-2	12/13/2010	90 cm.	6.1	5.93 ± 0.73	4.27 - 7.93	Pass
<u>Environmental, Inc.</u>						
2011-1	7/6/2011	100 cm.	6.71	5.64 ± 0.30	4.70 - 8.72	Pass
2011-1	7/6/2011	110 cm.	5.54	4.60 ± 0.46	3.88 - 7.20	Pass
2011-1	7/6/2011	120 cm.	4.66	4.68 ± 0.29	3.26 - 6.06	Pass
2011-1	7/6/2011	150 cm.	2.98	2.93 ± 0.66	2.09 - 3.87	Pass
2011-1	7/6/2011	180 cm.	2.07	2.05 ± 0.18	1.45 - 2.69	Pass
2011-1	7/6/2011	40 cm.	41.92	52.36 ± 3.08	29.34 - 54.50	Pass
2011-1	7/6/2011	45 cm.	33.12	41.83 ± 3.46	23.18 - 43.06	Pass
2011-1	7/6/2011	50 cm.	26.83	28.61 ± 2.63	18.78 - 34.88	Pass
2011-1	7/6/2011	60 cm.	18.63	21.00 ± 1.15	13.04 - 24.22	Pass
2011-1	7/6/2011	70 cm.	13.69	13.24 ± 1.76	9.58 - 17.80	Pass
2011-1	7/6/2011	80 cm.	10.48	12.18 ± 0.65	7.34 - 13.62	Pass
2011-1	7/6/2011	90 cm.	8.28	7.95 ± 0.82	5.80 - 10.76	Pass

TABLE A-3. In-House "Spike" Samples

Lab Code ^b	Date	Analysis	Concentration (pCi/L) ^a			Acceptance
			Laboratory results 2s, n=1 ^c	Known Activity	Control Limits ^d	
SPW-202	1/17/2011	U-238	4.19 ± 0.19	4.17	0.00 - 16.17	Pass
W-20111	2/1/2011	Ra-226	16.32 ± 0.47	16.77	11.74 - 21.80	Pass
W-20711	2/7/2011	Gr. Alpha	23.02 ± 0.45	20.00	10.00 - 30.00	Pass
W-20711	2/7/2011	Gr. Beta	46.59 ± 0.41	45.20	35.20 - 55.20	Pass
XWW-331	2/11/2011	Ba-133	144.30 ± 8.50	144.40	129.96 - 158.84	Pass
XWW-331	2/11/2011	Cs-134	22.20 ± 3.70	21.50	11.50 - 31.50	Pass
XWW-331	2/11/2011	Cs-137	64.70 ± 7.40	61.00	51.00 - 71.00	Pass
XWW-331	2/11/2011	H-3	13399 ± 334	12538	10030 - 15046	Pass
SPAP-567	2/14/2011	Gr. Beta	46.90 ± 0.11	48.10	28.86 - 67.34	Pass
SPAP-569	2/14/2011	Cs-134	7.70 ± 1.70	7.49	0.00 - 17.49	Pass
SPAP-569	2/14/2011	Cs-137	102.47 ± 3.20	106.79	96.11 - 117.47	Pass
SPAP-571	2/14/2011	H-3	75815 ± 542	73230	58584 - 87876	Pass
SPW-581	2/15/2011	Cs-134	39.91 ± 1.38	37.45	27.45 - 47.45	Pass
SPW-581	2/15/2011	Cs-137	56.28 ± 2.28	53.39	43.39 - 63.39	Pass
SPW-581	2/15/2011	Sr-89	112.92 ± 5.61	121.42	97.14 - 145.70	Pass
SPW-581	2/15/2011	Sr-90	47.80 ± 2.02	42.07	33.66 - 50.48	Pass
SPMI-583	2/15/2011	Cs-137	57.04 ± 2.76	53.39	43.39 - 63.39	Pass
SPMI-583	2/15/2011	Sr-90	36.27 ± 1.47	42.07	33.66 - 50.48	Pass
SPW-602	2/17/2011	U-238	3.98 ± 0.19	4.17	0.00 - 16.17	Pass
SPW-686	2/25/2011	Ni-63	167.41 ± 3.05	208.11	145.68 - 270.54	Pass
SPF-1113	3/17/2011	Cs-137	2369 ± 22	2170	1953 - 2387	Pass
XWW-1602	3/21/2011	Ba-133	26.83 ± 6.35	28.58	18.58 - 38.58	Pass
XWW-1602	3/21/2011	Cs-134	18.90 ± 4.06	16.30	6.30 - 26.30	Pass
XWW-1602	3/21/2011	Cs-137	33.98 ± 5.88	30.50	20.50 - 40.50	Pass
XWW-1602	3/21/2011	H-3	7348 ± 248	7617	6094 - 9140	Pass
XWW-2537	4/4/2011	Ba-133	43.40 ± 4.26	42.70	32.70 - 52.70	Pass
XWW-2537	4/4/2011	Cs-134	13.50 ± 2.40	11.90	1.90 - 21.90	Pass
XWW-2537	4/4/2011	Cs-137	68.30 ± 5.90	60.70	50.70 - 70.70	Pass
XWW-2537	4/4/2011	H-3	7134 ± 257	7234	5787 - 8681	Pass
SPW-2877	5/3/2011	Ra-228	25.23 ± 2.48	31.62	22.13 - 41.11	Pass
SPMI-3167	5/24/2011	Cs-134	33.04 ± 8.25	34.19	24.19 - 44.19	Pass
SPMI-3167	5/24/2011	Cs-137	51.53 ± 8.63	53.06	43.06 - 63.06	Pass
SPMI-3167	5/24/2011	Sr-89	90.89 ± 4.30	93.47	74.78 - 112.16	Pass
SPMI-3167	5/24/2011	Sr-90	41.17 ± 1.53	41.80	33.44 - 50.16	Pass
W-52411	5/24/2011	Ra-226	17.90 ± 0.42	16.80	11.76 - 21.84	Pass
W-60711	6/7/2011	Gr. Alpha	23.00 ± 0.49	20.00	10.00 - 30.00	Pass
W-60711	6/7/2011	Gr. Beta	43.27 ± 0.42	45.20	35.20 - 55.20	Pass
SPAP-4167	7/7/2011	Cs-134	6.92 ± 1.45	6.57	0.00 - 16.57	Pass
SPAP-4167	7/7/2011	Cs-137	108.02 ± 2.84	105.80	95.22 - 116.38	Pass
SPW-4169	7/7/2011	Cs-134	34.52 ± 4.79	32.84	22.84 - 42.84	Pass
SPW-4169	7/7/2011	Cs-137	58.29 ± 6.19	52.92	42.92 - 62.92	Pass

TABLE A-3. In-House "Spike" Samples

Lab Code ^b	Date	Analysis	Concentration (pCi/L) ^a			Acceptance
			Laboratory results 2s, n=1 ^c	Known Activity	Control Limits ^d	
SPW-4169	7/7/2011	Sr-89	66.12 ± 4.18	69.64	55.71 - 83.57	Pass
SPW-4169	7/7/2011	Sr-90	41.72 ± 1.79	41.68	33.34 - 50.02	Pass
SPW-4171	7/7/2011	H-3	70582 ± 767	71646	57317 - 85975	Pass
SPW-4180	7/7/2011	Tc-99	95.69 ± 1.65	97.02	67.91 - 126.13	Pass
SPW-41821	7/7/2011	Ra-228	32.57 ± 2.63	30.63	21.44 - 39.82	Pass
SPW-4241	7/7/2011	Ni-63	403.01 ± 4.66	415.20	290.64 - 539.76	Pass
SPW-4180	7/8/2011	Tc-99	100.30 ± 1.75	97.02	67.91 - 126.13	Pass
SPW-5029	7/29/2011	C-14	3991 ± 17	4739	2843 - 6634	Pass
SPW-5031	7/29/2011	Fe-55	13801 ± 331	14895	11916 - 17874	Pass
W-91411	9/14/2011	Gr. Alpha	21.58 ± 0.44	20.00	10.00 - 30.00	Pass
W-91411	9/14/2011	Gr. Beta	43.02 ± 0.40	45.20	35.20 - 55.20	Pass
SPW-91511	9/15/2011	Tc-99	29.92 ± 1.07	32.34	20.34 - 44.34	Pass
W-91911	9/19/2011	Ra-226	17.06 ± 0.42	16.80	11.76 - 21.84	Pass
W-100711	10/7/2011	Gr. Alpha	22.05 ± 0.45	20.00	10.00 - 30.00	Pass
W-100711	10/7/2011	Gr. Beta	45.51 ± 0.41	45.20	35.20 - 55.20	Pass
W-101111	10/11/2011	Ra-226	16.02 ± 0.40	16.80	11.76 - 21.84	Pass
XWW-7220	11/17/2011	Ba-133	25.11 ± 4.36	27.47	17.47 - 37.47	Pass
XWW-7220	11/17/2011	Cs-134	14.09 ± 3.11	16.60	6.60 - 26.60	Pass
XWW-7220	11/17/2011	Cs-137	35.59 ± 4.28	29.98	19.98 - 39.98	Pass
W-113011	11/30/2011	Ra-226	16.12 ± 0.39	16.80	11.76 - 21.84	Pass
W-120111	12/1/2011	Gr. Alpha	21.34 ± 0.43	20.00	10.00 - 30.00	Pass
W-120111	12/1/2011	Gr. Beta	45.55 ± 0.41	45.20	35.20 - 55.20	Pass
SPW-41823	12/9/2011	Ra-228	26.98 ± 2.38	29.40	20.58 - 38.22	Pass
SPMI-8906	12/22/2011	Cs-134	29.11 ± 3.52	28.14	18.14 - 38.14	Pass
SPMI-8906	12/22/2011	Cs-137	58.27 ± 7.62	52.36	42.36 - 62.36	Pass
SPW-8916	12/22/2011	Cs-134	31.74 ± 3.63	28.14	18.14 - 38.14	Pass
SPW-8916	12/22/2011	Cs-137	56.48 ± 6.12	52.36	42.36 - 62.36	Pass
SPAP-8902	12/23/2011	Gr. Beta	45.72 ± 0.11	47.11	28.27 - 65.95	Pass
SPAP-8904	12/23/2011	Cs-134	5.19 ± 0.63	5.63	0.00 - 15.63	Pass
SPAP-8904	12/23/2011	Cs-137	101.21 ± 2.55	104.71	94.24 - 115.18	Pass
SPW-8918	12/23/2011	H-3	136759 ± 1056	137638	110110 - 165166	Pass
SPW-8922	12/23/2011	Ni-63	202.21 ± 3.75	206.88	144.82 - 268.94	Pass
SPW-8924	12/23/2011	Tc-99	126.10 ± 1.86	129.36	90.55 - 168.17	Pass
SPF-8926	12/23/2011	Cs-134	0.34 ± 0.01	0.33	0.20 - 0.47	Pass
SPF-8926	12/23/2011	Cs-137	2.34 ± 0.02	2.09	1.25 - 2.93	Pass

^a Liquid sample results are reported in pCi/Liter, air filters (pCi/filter), charcoal (pCi/m³), and solid samples (pCi/g).

^b Laboratory codes as follows: W (water), MI (milk), AP (air filter), SO (soil), VE (vegetation), CH (charcoal canister), F (fish), U (urine).

^c Results are based on single determinations.

^d Control limits are established from the precision values listed in Attachment A of this report, adjusted to ± 2σ.

NOTE: For fish, Jello is used for the Spike matrix. For Vegetation, cabbage is used for the Spike matrix.

TABLE A-4. In-House "Blank" Samples

Lab Code	Sample Type	Date	Analysis ^b	Concentration (pCi/L) ^a		
				Laboratory results (4.66σ)		Acceptance Criteria (4.66 σ)
				LLD	Activity ^c	
SPW-202	Water	1/17/2011	U-238	0.10	0.12 ± 0.12	1
W-20111	Water	2/1/2011	Ra-226	0.04	0.05 ± 0.03	1
W-20711	Water	2/7/2011	Gr. Alpha	0.44	-0.02 ± 0.29	1
W-20711	Water	2/7/2011	Gr. Beta	0.75	-0.03 ± 0.53	3.2
SPAP-566	Air Filter	2/14/2011	Gr. Beta	0.64	2.24 ± 0.61	3.2
SPAP-568	Air Filter	2/14/2011	Cs-134	2.34	-	100
SPAP-568	Air Filter	2/14/2011	Cs-137	1.56	-	100
SPAP-570	Air Filter	2/14/2011	H-3	103.20	-49.40 ± 52.50	200
SPW-580	Water	2/15/2011	Cs-134	2.68	-	10
SPW-580	Water	2/15/2011	Cs-137	2.84	-	10
SPW-580	Water	2/15/2011	Sr-89	0.73	0.24 ± 0.57	5
SPW-580	Water	2/15/2011	Sr-90	0.57	0.02 ± 0.27	1
SPMI-582	Milk	2/15/2011	Cs-134	3.49	-	10
SPMI-582	Milk	2/15/2011	Cs-137	3.54	-	10
SPMI-582	Milk	2/15/2011	I-131(G)	4.14	-	20
SPMI-582	Milk	2/15/2011	Sr-89	0.71	0.16 ± 0.67	5
SPMI-582	Milk	2/15/2011	Sr-90	0.55	0.59 ± 0.32	1
SPW-601	Water	2/17/2011	U-238	0.20	0.09 ± 0.17	1
SPW-685	Water	2/25/2011	Ni-63	1.61	0.05 ± 0.98	20
SPF-1112	Fish	3/17/2011	Cs-134	6.74	-	100
SPF-1112	Fish	3/17/2011	Cs-137	5.45	-	100
BKW-40111	Water	4/1/2011	I-131	4.16	-	10
BKW-40111	Water	4/1/2011	Co-60	3.11	-	10
BKW-40111	Water	4/1/2011	Cs-134	4.73	-	10
BKW-40111	Water	4/1/2011	Cs-137	5.04	-	10
SPW-2887	Water	5/3/2011	Ra-228	0.72	0.46 ± 0.39	2
W-52411	Water	5/24/2011	Ra-226	0.04	0.05 ± 0.03	1
W-60711	Water	6/7/2011	Gr. Alpha	0.51	0.00 ± 0.36	1
W-60711	Water	6/7/2011	Gr. Beta	1.58	0.38 ± 1.12	3.2
SPAP-4164	Air Filter	7/7/2011	Gr. Beta	0.72	1.04 ± 0.48	3.2
SPW-4168	Water	7/7/2011	Cs-134	3.41	-	10
SPW-4168	Water	7/7/2011	Cs-137	2.45	-	10
SPW-4168	Water	7/7/2011	Sr-89	0.72	0.40 ± 0.50	5
SPW-4168	Water	7/7/2011	Sr-90	0.51	-0.19 ± 0.21	1
SPW-4171	Water	7/7/2011	H-3	152.00	37.10 ± 81.80	200
SPW-41811	Water	7/7/2011	Ra-228	0.77	0.51 ± 0.42	2

TABLE A-4. In-House "Blank" Samples

Lab Code	Sample Type	Date	Analysis ^b	Concentration (pCi/L) ^a		
				Laboratory results (4.66 σ)		Acceptance Criteria (4.66 σ)
				LLD	Activity ^c	
SPW-4241	Water	7/7/2011	Ni-63	1.70	0.09 \pm 1.03	20
SPW-4179	Water	7/8/2011	Tc-99	1.20	-0.96 \pm 0.71	10
SPW-5028	Water	7/29/2011	C-14	109.80	61.90 \pm 59.20	200
SPW-5031	Water	7/29/2011	Fe-55	140.60	0.00 \pm 85.30	1000
W-91411	Water	9/14/2011	Gr. Alpha	0.48	-0.06 \pm 0.33	1
W-91411	Water	9/14/2011	Gr. Beta	0.78	-0.43 \pm 0.53	3.2
SPW-91511	Water	9/15/2011	Tc-99	1.11	-0.62 \pm 0.66	10
W-91911	Water	9/19/2011	Ra-226	0.03	0.04 \pm 0.02	1
W-100711	Water	10/7/2011	Gr. Alpha	0.44	-0.26 \pm 0.28	1
W-100711	Water	10/7/2011	Gr. Beta	0.76	-0.43 \pm 0.52	3.2
W-101111	Water	10/11/2011	Ra-226	0.04	0.05 \pm 0.03	1
W-113011	Water	11/30/2011	Ra-226	0.03	0.04 \pm 0.02	1
W-120111	Water	12/1/2011	Gr. Alpha	0.41	-0.20 \pm 0.27	1
W-120111	Water	12/1/2011	Gr. Beta	0.75	-0.10 \pm 0.53	3.2
SPW-41813	Water	12/9/2011	Ra-228	0.71	0.17 \pm 0.35	2
SPMI-8905	Milk	12/22/2011	Cs-134	3.27	-	10
SPMI-8905	Milk	12/22/2011	Cs-137	3.38	-	10
SPMI-8905	Milk	12/22/2011	I-131(G)	2.17	-	20
SPW-8915	Water	12/22/2011	Cs-134	3.37	-	10
SPW-8915	Water	12/22/2011	Cs-137	3.45	-	10
SPW-8915	Water	12/22/2011	I-131(G)	3.38	-	20
SPAP-8901	Air Filter	12/23/2011	Gr. Beta	0.78	0.50 \pm 0.46	3.2
SPAP-8903	Air Filter	12/23/2011	Cs-134	1.65	-	100
SPAP-8903	Air Filter	12/23/2011	Cs-137	2.41	-	100
SPW-8917	Water	12/23/2011	H-3	150.20	-3.04 \pm 78.80	200
SPW-8921	Water	12/23/2011	Ni-63	16.92	-4.60 \pm 10.16	20
SPW-8923	Water	12/23/2011	Tc-99	5.66	-5.45 \pm 3.34	10
SPF-8925	Fish	12/23/2011	Cs-134	7.15	-	100
SPF-8925	Fish	12/23/2011	Cs-137	9.73	-	100

^a Liquid sample results are reported in pCi/Liter, air filters(pCi/filter), charcoal (pCi/charcoal canister), and solid samples (pCi/kg).

^b I-131(G); iodine-131 as analyzed by gamma spectroscopy.

^c Activity reported is a net activity result. For gamma spectroscopic analysis, activity detected below the LLD value is not reported.

TABLE A-5. In-House "Duplicate" Samples

Lab Code	Date	Analysis	Concentration (pCi/L) ^a			Acceptance
			First Result	Second Result	Averaged Result	
CF-20, 21	1/3/2011	Be-7	0.24 ± 0.14	0.34 ± 0.17	0.29 ± 0.11	Pass
CF-20, 21	1/3/2011	K-40	10.37 ± 0.43	9.76 ± 0.68	10.07 ± 0.40	Pass
CF-20, 21	1/3/2011	Sr-90	0.01 ± 0.01	0.01 ± 0.01	0.01 ± 0.00	Pass
WW-65, 66	1/6/2011	H-3	321.91 ± 97.19	345.76 ± 98.16	333.83 ± 69.06	Pass
BS-165, 166	1/11/2011	Cs-137	0.13 ± 0.02	0.15 ± 0.02	0.14 ± 0.01	Pass
BS-165, 166	1/11/2011	H-3	286.00 ± 80.00	284.00 ± 80.00	285.00 ± 56.57	Pass
BS-165, 166	1/11/2011	K-40	14.11 ± 0.52	13.79 ± 0.60	13.95 ± 0.40	Pass
BS-176, 177	1/11/2011	H-3	391.00 ± 92.00	332.00 ± 89.00	361.50 ± 64.00	Pass
BS-176, 177	1/11/2011	K-40	9.06 ± 0.44	8.28 ± 0.81	8.67 ± 0.46	Pass
BS-197, 198	1/11/2011	Cs-137	0.14 ± 0.03	0.15 ± 0.04	0.15 ± 0.03	Pass
BS-197, 198	1/11/2011	H-3	459.00 ± 103.00	283.00 ± 95.00	371.00 ± 70.06	Pass
BS-197, 198	1/11/2011	K-40	14.40 ± 0.77	14.16 ± 1.23	14.28 ± 0.73	Pass
WW-358, 359	1/17/2011	H-3	331.44 ± 93.05	407.65 ± 95.91	369.55 ± 66.81	Pass
DW-20009, 20010	1/19/2011	Ra-226	3.66 ± 0.57	2.74 ± 0.43	3.20 ± 0.36	Pass
DW-20009, 20010	1/19/2011	Ra-228	1.51 ± 0.64	1.36 ± 0.60	1.44 ± 0.44	Pass
WW-337, 338	1/25/2011	H-3	21986.00 ± 402.00	21896.00 ± 401.00	21941.00 ± 283.90	Pass
W-491, 492	1/27/2011	Ra-226	6.70 ± 0.50	6.10 ± 0.50	6.40 ± 0.35	Pass
W-491, 492	1/27/2011	Ra-228	6.60 ± 1.30	8.40 ± 1.40	7.50 ± 0.96	Pass
DW-20014, 20015	1/28/2011	Gr. Alpha	1.91 ± 0.71	2.34 ± 0.80	2.13 ± 0.53	Pass
SWU-447, 448	1/31/2011	Gr. Beta	7.42 ± 1.17	6.85 ± 1.11	7.14 ± 0.81	Pass
W-694, 695	2/7/2011	H-3	628.26 ± 104.30	692.37 ± 106.89	660.32 ± 74.67	Pass
DW-20022, 20023	2/9/2011	Ra-228	0.71 ± 0.47	1.13 ± 0.54	0.92 ± 0.36	Pass
SW-626, 627	2/16/2011	H-3	1268.17 ± 129.52	1144.65 ± 125.39	1206.41 ± 90.14	Pass
LW-825, 826	2/24/2011	Gr. Beta	2.65 ± 0.82	2.45 ± 0.74	2.55 ± 0.55	Pass
SWT-845, 846	3/1/2011	Gr. Beta	1.11 ± 0.39	0.80 ± 0.37	0.96 ± 0.27	Pass
MI-998, 999	3/7/2011	K-40	1760.10 ± 127.50	1708.50 ± 131.60	1734.30 ± 91.62	Pass
W-1024, 1025	3/7/2011	H-3	489.83 ± 101.09	581.39 ± 105.06	535.61 ± 72.90	Pass
WW-1156, 1157	3/16/2011	Gr. Beta	1.79 ± 0.78	0.47 ± 0.66	1.13 ± 0.51	Pass
P-1198, 1199	3/17/2011	H-3	504.00 ± 133.00	597.00 ± 136.00	550.50 ± 95.11	Pass
SW-1434, 1435	3/28/2011	H-3	15523.00 ± 359.00	15968.00 ± 364.00	15745.50 ± 255.63	Pass
WW-1588, 1589	3/28/2011	Gr. Beta	1.81 ± 1.23	2.81 ± 1.38	2.31 ± 0.92	Pass
SG-1714, 1715	3/28/2011	Gr. Alpha	8.82 ± 0.81	8.58 ± 0.74	8.70 ± 0.55	Pass
SG-1714, 1715	3/28/2011	Gr. Beta	13.78 ± 0.65	12.76 ± 0.58	13.27 ± 0.44	Pass
AP-1862, 1863	3/28/2011	Be-7	0.09 ± 0.02	0.08 ± 0.02	0.08 ± 0.01	Pass
W-2143, 2144	3/28/2011	H-3	536.40 ± 99.37	466.79 ± 96.46	501.59 ± 69.25	Pass
AP-2269, 2270	3/28/2011	Be-7	0.07 ± 0.01	0.08 ± 0.01	0.07 ± 0.01	Pass
DW-20061, 20062	3/28/2011	Gr. Alpha	2.82 ± 1.33	3.89 ± 1.26	3.36 ± 0.92	Pass
SWU-1455, 1456	3/29/2011	Gr. Beta	2.50 ± 0.75	2.75 ± 0.83	2.62 ± 0.56	Pass
SWU-1522, 1523	3/29/2011	Gr. Beta	1.36 ± 0.87	2.14 ± 0.96	1.75 ± 0.65	Pass
PM-1543, 1544	3/29/2011	Gr. Beta	13.81 ± 0.26	13.67 ± 0.27	13.74 ± 0.19	Pass
PM-1543, 1544	3/29/2011	Sr-90	8.12 ± 3.20	7.71 ± 3.25	7.91 ± 2.28	Pass

TABLE A-5. In-House "Duplicate" Samples

Lab Code	Date	Analysis	Concentration (pCi/L) ^a			Acceptance
			First Result	Second Result	Averaged Result	
SWT-5885, 5886	3/29/2011	Gr. Beta	1.21 ± 0.54	0.77 ± 0.54	0.99 ± 0.38	Pass
AP-1883, 1884	3/30/2011	Be-7	0.07 ± 0.01	0.09 ± 0.02	0.08 ± 0.01	Pass
AP-2248, 2249	3/30/2011	Be-7	0.06 ± 0.01	0.06 ± 0.01	0.06 ± 0.01	Pass
DW-20066, 20067	3/30/2011	Ra-226	2.14 ± 0.16	2.10 ± 0.16	2.12 ± 0.11	Pass
DW-20066, 20067	3/30/2011	Ra-228	2.55 ± 0.65	1.78 ± 0.62	2.17 ± 0.45	Pass
P-1567, 1568	4/1/2011	H-3	289.00 ± 103.00	296.00 ± 103.00	292.50 ± 72.83	Pass
MI-1609, 1610	4/4/2011	I-131	0.85 ± 0.17	0.91 ± 0.18	0.88 ± 0.13	Pass
MI-1609, 1610	4/4/2011	K-40	1323.80 ± 112.00	1323.20 ± 96.22	1323.50 ± 73.83	Pass
MI-1609, 1610	4/4/2011	Sr-90	0.85 ± 0.33	0.97 ± 0.34	0.91 ± 0.24	Pass
S-1651, 1652	4/4/2011	Ac-228	0.88 ± 0.08	1.03 ± 0.22	0.96 ± 0.12	Pass
S-1651, 1652	4/4/2011	Pb-214	1.09 ± 0.12	0.84 ± 0.16	0.97 ± 0.10	Pass
AP-1841, 1842	4/7/2011	Be-7	0.12 ± 0.02	0.12 ± 0.01	0.12 ± 0.01	Pass
AP-1841, 1842	4/7/2011	Cs-137	0.00 ± 0.00	0.00 ± 0.00	0.00 ± 0.00	Pass
AP-1841, 1842	4/7/2011	I-131(G)	0.02 ± 0.00	0.03 ± 0.00	0.03 ± 0.00	Pass
S-1990, 1991	4/7/2011	Ac-228	15.83 ± 0.39	16.12 ± 0.64	15.98 ± 0.37	Pass
S-1990, 1991	4/7/2011	Pb-214	11.21 ± 0.23	11.81 ± 1.22	11.51 ± 0.62	Pass
WW-2552, 2553	4/7/2011	H-3	761.09 ± 116.48	759.04 ± 116.41	760.07 ± 82.34	Pass
PM-1904, 1905	4/11/2011	K-40	13585.00 ± 611.00	14278.00 ± 648.00	13931.50 ± 445.32	Pass
PM-1904, 1905	4/11/2011	Sr-90	9.94 ± 3.05	5.62 ± 2.52	7.78 ± 1.98	Pass
P-2011, 2012	4/11/2011	H-3	670.00 ± 108.00	619.00 ± 106.00	644.50 ± 75.66	Pass
WW-2053, 2054	4/13/2011	H-3	220.20 ± 86.50	246.80 ± 87.80	233.50 ± 61.63	Pass
BS-2095, 2096	4/13/2011	K-40	12.88 ± 0.72	13.56 ± 1.08	13.22 ± 0.65	Pass
DW-20099, 20100	4/13/2011	U-233/4	1.64 ± 0.40	1.31 ± 0.34	1.48 ± 0.26	Pass
DW-20099, 20100	4/13/2011	U-238	1.49 ± 0.39	1.28 ± 0.33	1.39 ± 0.26	Pass
WW-2416, 2417	4/19/2011	H-3	217.10 ± 97.00	184.90 ± 95.60	201.00 ± 68.10	Pass
P-2185, 2186	4/20/2011	H-3	405.00 ± 93.00	504.00 ± 98.00	454.50 ± 67.55	Pass
WW-2353, 2354	4/20/2011	H-3	525.54 ± 119.74	399.41 ± 115.99	462.48 ± 83.35	Pass
DW-20115, 20116	4/26/2011	U-233/4	11.94 ± 2.34	10.71 ± 1.19	11.33 ± 1.31	Pass
DW-20115, 20116	4/26/2011	U-238	2.70 ± 1.15	3.89 ± 0.72	3.30 ± 0.68	Pass
SO-2960, 2961	4/27/2011	K-40	22.63 ± 1.36	22.90 ± 0.03	22.77 ± 0.68	Pass
MI-2657, 2658	5/2/2011	K-40	1319.30 ± 101.30	1403.20 ± 131.60	1361.25 ± 83.04	Pass
DW-20130, 20131	5/2/2011	U-233/4	7.59 ± 0.90	7.62 ± 0.83	7.61 ± 0.61	Pass
DW-20130, 20131	5/2/2011	U-238	4.67 ± 0.72	4.84 ± 0.66	4.76 ± 0.49	Pass
DW-20148, 20149	5/3/2011	U-233/4	6.64 ± 0.83	6.35 ± 0.81	6.50 ± 0.58	Pass
DW-20148, 20149	5/3/2011	U-238	6.11 ± 0.83	5.18 ± 0.73	5.65 ± 0.55	Pass
PM-2810, 2811	5/4/2011	Cs-134	18.64 ± 12.16	33.33 ± 11.86	25.99 ± 8.49	Pass
PM-2810, 2811	5/4/2011	Cs-137	28.99 ± 14.92	21.17 ± 12.16	25.08 ± 9.62	Pass
PM-2810, 2811	5/4/2011	K-40	14368.00 ± 720.00	14309.00 ± 638.00	14338.50 ± 481.00	Pass
WW-3065, 3066	5/16/2011	H-3	280.51 ± 86.98	179.46 ± 82.83	229.98 ± 60.05	Pass
WW-3086, 3087	5/16/2011	H-3	341.14 ± 85.94	377.97 ± 87.43	359.56 ± 61.30	Pass

TABLE A-5. In-House "Duplicate" Samples

Lab Code	Date	Analysis	Concentration (pCi/L) ^a			Acceptance
			First Result	Second Result	Averaged Result	
SG-3134, 3135	5/16/2011	Ac-228	11.19 ± 0.82	12.50 ± 0.84	11.85 ± 0.59	Pass
SG-3134, 3135	5/16/2011	Pb-214	9.12 ± 0.17	9.37 ± 0.42	9.25 ± 0.23	Pass
F-3221, 3222	5/23/2011	K-40	2.73 ± 0.39	2.81 ± 0.42	2.77 ± 0.29	Pass
SS-3434, 3435	5/25/2011	K-40	11533.00 ± 563.70	11236.00 ± 566.10	11384.50 ± 399.45	Pass
AP-3329, 3330	5/26/2011	Be-7	0.24 ± 0.11	0.23 ± 0.13	0.24 ± 0.08	Pass
WW-3350, 3351	6/1/2011	H-3	235.37 ± 83.98	173.12 ± 81.05	204.25 ± 58.36	Pass
G-3413, 3414	6/1/2011	Be-7	0.28 ± 0.10	0.25 ± 0.09	0.27 ± 0.07	Pass
G-3413, 3414	6/1/2011	Gr. Beta	11.04 ± 0.31	10.85 ± 0.31	10.95 ± 0.22	Pass
G-3413, 3414	6/1/2011	K-40	6.80 ± 0.33	6.71 ± 0.38	6.76 ± 0.25	Pass
AP-3602, 3603	6/3/2011	Be-7	0.20 ± 0.08	0.25 ± 0.10	0.22 ± 0.07	Pass
SO-3797, 3798	6/8/2011	Ac-228	0.99 ± 0.05	1.00 ± 0.06	1.00 ± 0.04	Pass
SO-3797, 3798	6/8/2011	Bi-212	1.10 ± 0.12	1.08 ± 0.17	1.09 ± 0.10	Pass
SO-3797, 3798	6/8/2011	Bi-214	0.87 ± 0.02	0.86 ± 0.02	0.87 ± 0.01	Pass
SO-3797, 3798	6/8/2011	Cs-137	0.41 ± 0.01	0.39 ± 0.01	0.40 ± 0.01	Pass
SO-3797, 3798	6/8/2011	K-40	16.08 ± 0.26	16.27 ± 0.29	16.18 ± 0.19	Pass
SO-3797, 3798	6/8/2011	Pb-212	0.98 ± 0.10	0.93 ± 0.02	0.96 ± 0.05	Pass
SO-3797, 3798	6/8/2011	Pb-214	0.95 ± 0.02	0.91 ± 0.02	0.93 ± 0.01	Pass
SO-3797, 3798	6/8/2011	Th-232	0.47 ± 0.05	0.49 ± 0.04	0.48 ± 0.03	Pass
SO-3797, 3798	6/8/2011	U-233/4	0.16 ± 0.02	0.15 ± 0.02	0.16 ± 0.01	Pass
SO-3797, 3798	6/8/2011	U-238	0.16 ± 0.02	0.13 ± 0.02	0.15 ± 0.01	Pass
MI-3935, 3936	6/20/2011	K-40	1764.60 ± 119.40	1843.10 ± 136.50	1803.85 ± 90.68	Pass
BS-4172, 4173	6/21/2011	Cs-137	51.50 ± 23.78	48.57 ± 17.06	50.04 ± 14.63	Pass
BS-4172, 4173	6/21/2011	K-40	11730.00 ± 679.60	11120.00 ± 512.30	11425.00 ± 425.53	Pass
DW-20183, 20184	6/21/2011	U-233/4	10.00 ± 1.00	8.40 ± 0.90	9.20 ± 0.67	Pass
DW-20183, 20184	6/21/2011	U-238	6.70 ± 0.80	6.10 ± 0.80	6.40 ± 0.57	Pass
WW-4019, 4020	6/24/2011	Gr. Beta	3.56 ± 1.20	3.16 ± 1.21	3.36 ± 0.85	Pass
PM-4193, 4194	6/30/2011	K-40	14795.00 ± 759.00	14660.00 ± 750.00	14727.50 ± 533.52	Pass
LW-4235, 4236	6/30/2011	Gr. Beta	2.70 ± 0.72	2.11 ± 0.78	2.41 ± 0.53	Pass
AP-4367, 4368	7/7/2011	Be-7	0.17 ± 0.10	0.19 ± 0.11	0.18 ± 0.07	Pass
MI-4416, 4417	7/11/2011	K-40	1342.40 ± 91.49	1447.00 ± 114.80	1394.70 ± 73.40	Pass
W-4914, 4915	7/11/2011	H-3	576.36 ± 110.35	584.67 ± 110.67	580.52 ± 78.14	Pass
MI-4438, 4439	7/12/2011	K-40	1280.60 ± 107.50	1381.20 ± 112.70	1330.90 ± 77.87	Pass
VE-4481, 4482	7/13/2011	K-40	4452.60 ± 332.40	4767.90 ± 349.70	4610.25 ± 241.24	Pass
AP-4677, 4678	7/15/2011	Be-7	0.18 ± 0.08	0.23 ± 0.09	0.20 ± 0.06	Pass
W-5537, 5538	7/18/2011	H-3	650.13 ± 105.19	695.39 ± 106.94	672.76 ± 75.00	Pass
P-4764, 4765	7/19/2011	H-3	179.82 ± 84.81	138.72 ± 82.79	159.27 ± 59.26	Pass
WW-5211, 5212	7/24/2011	H-3	191.94 ± 85.50	136.22 ± 82.76	164.08 ± 59.50	Pass

TABLE A-5. In-House "Duplicate" Samples

Lab Code	Date	Analysis	Concentration (pCi/L) ^a			Acceptance
			First Result	Second Result	Averaged Result	
VE-4998, 4999	7/25/2011	Be-7	543.90 ± 158.20	488.30 ± 163.80	516.10 ± 113.86	Pass
VE-4998, 4999	7/25/2011	K-40	2562.20 ± 319.80	2414.00 ± 350.00	2488.10 ± 237.05	Pass
DW-20258, 20259	7/25/2011	U-233/4	21.34 ± 1.52	24.93 ± 2.93	23.14 ± 1.65	Pass
DW-20258, 20259	7/25/2011	U-235	0.57 ± 0.26	0.69 ± 0.26	0.63 ± 0.18	Pass
DW-20258, 20259	7/25/2011	U-238	14.11 ± 1.24	15.81 ± 1.23	14.96 ± 0.87	Pass
DW-20269, 20270	7/25/2011	U-233/4	4.93 ± 0.73	4.65 ± 0.68	4.79 ± 0.50	Pass
DW-20269, 20270	7/25/2011	U-238	3.26 ± 0.60	2.53 ± 0.50	2.90 ± 0.39	Pass
DW-20280, 20281	7/25/2011	U-233/4	3.58 ± 0.58	3.33 ± 0.56	3.46 ± 0.40	Pass
DW-20280, 20281	7/25/2011	U-238	1.64 ± 0.40	2.11 ± 0.45	1.88 ± 0.30	Pass
MI-5019, 5020	7/26/2011	K-40	1348.50 ± 101.00	1347.40 ± 109.70	1347.95 ± 74.56	Pass
W-5447, 5448	7/26/2011	H-3	246.31 ± 99.19	241.99 ± 99.02	244.15 ± 70.08	Pass
G-5124, 5125	7/28/2011	Gr. Beta	7.48 ± 0.20	7.17 ± 0.19	7.33 ± 0.14	Pass
AP-5232, 5233	7/28/2011	Be-7	0.15 ± 0.08	0.22 ± 0.13	0.19 ± 0.08	Pass
SL-5169, 5170	8/1/2011	Be-7	2.37 ± 0.16	2.17 ± 0.17	2.27 ± 0.12	Pass
SL-5169, 5170	8/1/2011	Gr. Beta	4.74 ± 0.45	3.94 ± 0.39	4.34 ± 0.30	Pass
SL-5169, 5170	8/1/2011	K-40	3.12 ± 0.16	2.96 ± 0.21	3.04 ± 0.13	Pass
G-5190, 5191	8/1/2011	Be-7	3.14 ± 0.30	3.44 ± 0.27	3.29 ± 0.20	Pass
G-5190, 5191	8/1/2011	Gr. Beta	8.07 ± 0.28	7.86 ± 0.27	7.97 ± 0.19	Pass
G-5190, 5191	8/1/2011	K-40	5.51 ± 0.46	5.57 ± 0.44	5.54 ± 0.32	Pass
DW-20291, 20292	8/2/2011	U-233/4	3.24 ± 0.54	2.60 ± 0.50	2.92 ± 0.37	Pass
DW-20291, 20292	8/2/2011	U-238	1.59 ± 0.38	2.00 ± 0.43	1.80 ± 0.29	Pass
SG-5342, 5343	8/5/2011	Ac-228	14.41 ± 0.36	14.13 ± 0.48	14.27 ± 0.30	Pass
SG-5342, 5343	8/5/2011	Bi-212	4.14 ± 0.65	4.73 ± 1.21	4.44 ± 0.69	Pass
SG-5342, 5343	8/5/2011	K-40	7.67 ± 0.92	7.95 ± 1.21	7.81 ± 0.76	Pass
SG-5342, 5343	8/5/2011	Pb-214	10.72 ± 0.21	10.67 ± 0.28	10.70 ± 0.18	Pass
SG-5342, 5343	8/5/2011	Tl-208	0.96 ± 0.06	1.00 ± 0.06	0.98 ± 0.04	Pass
MI-5405, 5406	8/8/2011	K-40	1545.30 ± 116.00	1388.00 ± 98.20	1466.65 ± 75.99	Pass
DW-20301, 20302	8/9/2011	Gr. Alpha	6.36 ± 1.09	5.30 ± 1.08	5.83 ± 0.77	Pass
DW-20301, 20302	8/9/2011	Gr. Beta	14.36 ± 0.92	13.51 ± 0.89	13.94 ± 0.64	Pass
DW-5603, 5604	8/16/2011	Ra-228	1.68 ± 0.88	2.26 ± 0.91	1.97 ± 0.63	Pass
VE-5753, 5754	8/22/2011	Be-7	0.78 ± 0.20	0.75 ± 0.23	0.77 ± 0.15	Pass
VE-5753, 5754	8/22/2011	K-40	6.16 ± 0.51	6.63 ± 0.57	6.40 ± 0.38	Pass
S-5801, 5802	8/29/2011	Ac-228	0.43 ± 0.09	0.38 ± 0.07	0.41 ± 0.06	Pass
S-5801, 5802	8/29/2011	K-40	6.54 ± 0.51	5.96 ± 0.49	6.25 ± 0.35	Pass
S-5801, 5802	8/29/2011	Pb-212	0.31 ± 0.03	0.36 ± 0.03	0.34 ± 0.02	Pass
S-5801, 5802	8/29/2011	Pb-214	0.28 ± 0.04	0.25 ± 0.04	0.27 ± 0.03	Pass
S-5801, 5802	8/29/2011	Tl-208	0.14 ± 0.02	0.12 ± 0.02	0.13 ± 0.01	Pass
S-5801, 5802	8/29/2011	U-235	0.05 ± 0.02	0.04 ± 0.01	0.05 ± 0.01	Pass
ME-5996, 5997	9/1/2011	Gr. Alpha	0.03 ± 0.02	0.03 ± 0.02	0.03 ± 0.01	Pass
ME-5996, 5997	9/1/2011	Gr. Beta	2.55 ± 0.07	2.62 ± 0.07	2.58 ± 0.05	Pass
ME-5996, 5997	9/1/2011	K-40	2.66 ± 0.35	2.24 ± 0.58	2.45 ± 0.34	Pass

TABLE A-5. In-House "Duplicate" Samples

Lab Code	Date	Analysis	Concentration (pCi/L) ^a			Acceptance
			First Result	Second Result	Averaged Result	
SL-6017, 6018	9/6/2011	Be-7	0.47 ± 0.17	0.51 ± 0.19	0.49 ± 0.13	Pass
SL-6017, 6018	9/6/2011	Gr. Beta	4.23 ± 0.16	3.94 ± 0.15	4.09 ± 0.11	Pass
SL-6017, 6018	9/6/2011	K-40	4.43 ± 0.55	4.24 ± 0.53	4.34 ± 0.38	Pass
VE-6038, 6039	9/7/2011	Sr-90	1.86 ± 0.98	2.30 ± 0.92	2.08 ± 0.67	Pass
SW-6059, 6060	9/8/2011	H-3	219.75 ± 97.52	177.41 ± 95.76	198.58 ± 68.34	Pass
VE-6302, 6303	9/13/2011	Be-7	0.76 ± 0.24	0.85 ± 0.20	0.81 ± 0.16	Pass
VE-6302, 6303	9/13/2011	Gr. Beta	27.00 ± 1.02	25.50 ± 0.95	26.25 ± 0.70	Pass
VE-6302, 6303	9/13/2011	H-3	6966.00 ± 249.00	6947.00 ± 249.00	6956.50 ± 176.07	Pass
VE-6302, 6303	9/13/2011	K-40	20.62 ± 0.68	20.63 ± 0.64	20.63 ± 0.47	Pass
W-7098, 7099	9/19/2011	H-3	586.61 ± 103.06	525.71 ± 100.63	556.16 ± 72.02	Pass
W-6407, 6408	9/20/2011	Ra-228	1.61 ± 0.94	0.79 ± 0.81	1.20 ± 0.62	Pass
MI-6479, 6480	9/27/2011	K-40	1384.10 ± 111.10	1411.40 ± 105.00	1397.75 ± 76.43	Pass
W-6579, 6580	9/27/2011	H-3	287.97 ± 99.68	285.95 ± 99.60	286.96 ± 70.45	Pass
AP-7015, 7016	9/27/2011	Be-7	0.08 ± 0.02	0.09 ± 0.02	0.08 ± 0.01	Pass
AP-6105, 6106	9/28/2011	Be-7	0.11 ± 0.02	0.09 ± 0.02	0.10 ± 0.01	Pass
LW-6603, 6604	9/28/2011	Gr. Beta	2.15 ± 1.04	1.65 ± 0.90	1.90 ± 0.69	Pass
AP-7056, 7057	9/29/2011	Be-7	0.08 ± 0.02	0.06 ± 0.01	0.07 ± 0.01	Pass
G-6730, 6731	10/3/2011	Be-7	4.24 ± 0.36	4.47 ± 0.37	4.36 ± 0.26	Pass
G-6730, 6731	10/3/2011	Gr. Beta	8.27 ± 0.33	7.93 ± 0.31	8.10 ± 0.23	Pass
G-6730, 6731	10/3/2011	K-40	6.46 ± 0.56	5.41 ± 0.50	5.94 ± 0.38	Pass
AP-7077, 7078	10/3/2011	Be-7	0.08 ± 0.01	0.07 ± 0.01	0.07 ± 0.01	Pass
AP-7077, 7078	10/3/2011	Be-7	0.08 ± 0.01	0.07 ± 0.01	0.07 ± 0.01	Pass
VE-6798, 6799	10/4/2011	K-40	11.76 ± 0.65	11.91 ± 0.62	11.84 ± 0.45	Pass
AP-6820, 6821	10/6/2011	Be-7	0.22 ± 0.08	0.18 ± 0.10	0.20 ± 0.06	Pass
W-7755, 7756	10/9/2011	H-3	261.92 ± 96.52	221.92 ± 94.80	241.92 ± 67.65	Pass
BS-7944, 7945	10/10/2011	Cs-137	291.17 ± 34.00	330.68 ± 36.40	310.93 ± 24.90	Pass
BS-7944, 7945	10/10/2011	K-40	14237.00 ± 686.40	15359.00 ± 703.80	14798.00 ± 491.55	Pass
BS-7140, 7141	10/13/2011	K-40	2.59 ± 0.35	2.58 ± 0.52	2.59 ± 0.31	Pass
AP-7168, 7169	10/13/2011	Be-7	0.25 ± 0.09	0.25 ± 0.11	0.25 ± 0.07	Pass
DW-20349, 20350	10/13/2011	U-233/4	1.77 ± 0.41	2.25 ± 0.77	2.01 ± 0.44	Pass
DW-20349, 20350	10/13/2011	U-238	0.28 ± 0.19	0.31 ± 0.33	0.30 ± 0.19	Pass
WW-7667, 7668	10/19/2011	H-3	1049.11 ± 116.32	1071.39 ± 117.10	1060.25 ± 82.53	Pass
WW-7381, 7382	10/21/2011	H-3	1904.40 ± 145.45	1813.62 ± 142.91	1859.01 ± 101.95	Pass
SS-7495, 7496	10/26/2011	K-40	10.16 ± 0.55	9.56 ± 0.49	9.86 ± 0.37	Pass
W-7516, 7517	10/27/2011	H-3	191.46 ± 84.47	224.05 ± 86.03	207.76 ± 60.28	Pass
VE-7537, 7538	10/28/2011	K-40	2.08 ± 0.23	2.41 ± 0.21	2.24 ± 0.16	Pass
MI-7622, 7623	10/31/2011	K-40	1386.20 ± 116.80	1407.90 ± 116.50	1397.05 ± 82.48	Pass
DW-20399, 20400	10/31/2011	U-233/4	5.70 ± 0.70	5.70 ± 0.70	5.70 ± 0.49	Pass
DW-20399, 20400	10/31/2011	U-238	3.10 ± 0.50	3.70 ± 0.70	3.40 ± 0.43	Pass
BS-7600, 7601	11/1/2011	Gr. Beta	6.83 ± 1.44	5.31 ± 1.35	6.07 ± 0.98	Pass

TABLE A-5. In-House "Duplicate" Samples

Lab Code	Date	Analysis	Concentration (pCi/L) ^a			Acceptance
			First Result	Second Result	Averaged Result	
SG-8471, 8472	11/1/2011	Gr. Alpha	13.63 ± 2.32	11.13 ± 2.00	12.38 ± 1.53	Pass
SG-8471, 8472	11/1/2011	Gr. Beta	20.30 ± 1.43	17.65 ± 1.42	18.98 ± 1.01	Pass
DW-20424, 20425	11/7/2011	U-233/4	5.90 ± 0.80	6.10 ± 0.80	6.00 ± 0.57	Pass
DW-20424, 20425	11/7/2011	U-235	0.10 ± 0.10	0.30 ± 0.20	0.20 ± 0.11	Pass
DW-20424, 20425	11/7/2011	U-238	4.30 ± 0.70	3.70 ± 0.60	4.00 ± 0.46	Pass
DW-20424, 20425	11/7/2011	U-238	10.30 ± 1.00	10.10 ± 1.00	10.20 ± 0.71	Pass
DW-20435, 20436	11/8/2011	U-233/4	11.00 ± 1.10	10.60 ± 0.80	10.80 ± 0.68	Pass
DW-20435, 20436	11/8/2011	U-238	5.90 ± 0.80	4.90 ± 0.60	5.40 ± 0.50	Pass
SG-7902, 7903	11/10/2011	Ac-228	21.38 ± 0.47	20.48 ± 0.52	20.93 ± 0.35	Pass
SG-7902, 7903	11/10/2011	K-40	9.72 ± 1.04	9.53 ± 0.92	9.63 ± 0.69	Pass
SG-7902, 7903	11/10/2011	Pb-212	3.99 ± 0.10	3.99 ± 0.10	3.99 ± 0.07	Pass
SG-7902, 7903	11/10/2011	Pb-214	9.15 ± 0.23	9.14 ± 0.21	9.15 ± 0.16	Pass
BS-8033, 8034	11/11/2011	Cs-137	0.03 ± 0.02	0.03 ± 0.02	0.03 ± 0.01	Pass
LW-8075, 8076	11/16/2011	Gr. Beta	1.93 ± 0.62	2.55 ± 0.64	2.24 ± 0.44	Pass
AP-8193, 8194	11/17/2011	Be-7	0.21 ± 0.11	0.26 ± 0.13	0.24 ± 0.08	Pass
F-8663, 8664	11/19/2011	Cs-137	0.03 ± 0.02	0.03 ± 0.02	0.03 ± 0.01	Pass
F-8663, 8664	11/19/2011	Gr. Beta	3.55 ± 0.10	3.71 ± 0.10	3.63 ± 0.07	Pass
F-8663, 8664	11/19/2011	K-40	3.04 ± 0.42	3.05 ± 0.35	3.05 ± 0.27	Pass
DW-20449, 20450	11/28/2011	U-233/4	0.70 ± 0.20	0.80 ± 0.20	0.75 ± 0.14	Pass
DW-20449, 20450	11/28/2011	U-238	0.60 ± 0.20	0.60 ± 0.20	0.60 ± 0.14	Pass
SWU-8388, 8389	11/29/2011	Gr. Beta	1.66 ± 0.57	1.65 ± 0.59	1.66 ± 0.41	Pass
AP-8841, 8842	12/15/2011	Be-7	0.23 ± 0.12	0.19 ± 0.09	0.21 ± 0.07	Pass
W-8886, 8887	12/15/2011	Gr. Alpha	0.83 ± 0.81	1.58 ± 0.99	1.21 ± 0.64	Pass
W-8886, 8887	12/15/2011	Gr. Beta	6.80 ± 1.25	5.94 ± 1.22	6.37 ± 0.87	Pass
W-8886, 8887	12/15/2011	Ra-226	0.23 ± 0.15	0.41 ± 0.16	0.32 ± 0.11	Pass
SO-8958, 8959	12/21/2011	K-40	14.58 ± 0.86	15.07 ± 0.87	14.83 ± 0.61	Pass
AP-8907, 8908	12/22/2011	Be-7	0.15 ± 0.06	0.11 ± 0.07	0.13 ± 0.05	Pass
AP-9196, 9197	12/28/2011	Be-7	0.06 ± 0.01	0.07 ± 0.01	0.06 ± 0.01	Pass
LW-9091, 9092	12/29/2011	Gr. Beta	1.97 ± 0.63	1.74 ± 0.60	1.86 ± 0.44	Pass

Note: Duplicate analyses are performed on every twentieth sample received in-house. Results are not listed for those analyses with activities that measure below the LLD.

^a Results are reported in units of pCi/L, except for air filters (pCi/Filter), food products, vegetation, soil, sediment (pCi/g).

TABLE A-6. Department of Energy's Mixed Analyte Performance Evaluation Program (MAPEP)^a.

Lab Code ^c	Date	Analysis	Laboratory result	Concentration ^b		Acceptance
				Known Activity	Control Limits ^d	
STW-1237 ^e	02/01/11	Am-241	0.35 ± 0.10	0.53	0.37 - 0.69	Fail
STW-1237	02/01/11	Co-57	< 0.2	0.00	-	Pass
STW-1237	02/01/11	Co-60	24.10 ± 0.40	24.60	17.20 - 32.00	Pass
STW-1237	02/01/11	Cs-134	19.80 ± 0.40	21.50	15.10 - 28.00	Pass
STW-1237	02/01/11	Cs-137	29.40 ± 0.50	29.40	20.60 - 38.20	Pass
STW-1237	02/01/11	H-3	238.90 ± 8.80	243.00	170.00 - 316.00	Pass
STW-1237	02/01/11	K-40	95.40 ± 3.10	91.00	64.00 - 118.00	Pass
STW-1237	02/01/11	Mn-54	32.50 ± 0.60	31.60	22.10 - 41.10	Pass
STW-1237	02/01/11	Ni-63	16.30 ± 0.60	18.60	13.00 - 24.20	Pass
STW-1237	02/01/11	Pu-238	1.11 ± 0.12	1.06	0.75 - 1.38	Pass
STW-1237	02/01/11	Pu-239/40	0.88 ± 0.12	0.81	0.57 - 1.05	Pass
STW-1237	02/01/11	Sr-90	8.70 ± 0.70	8.72	6.10 - 11.34	Pass
STW-1237	02/01/11	Tc-99	7.60 ± 0.60	8.99	6.29 - 11.69	Pass
STW-1237	02/01/11	Zn-65	< 0.5	0.00	-	Pass
STW-1238	02/01/11	Gr. Alpha	0.82 ± 0.07	1.14	0.34 - 1.93	Pass
STW-1238	02/01/11	Gr. Beta	2.82 ± 0.07	2.96	1.48 - 4.44	Pass
STVE-1239	02/01/11	Co-57	11.27 ± 0.21	9.94	6.96 - 12.92	Pass
STVE-1239	02/01/11	Co-60	4.95 ± 0.16	4.91	3.44 - 6.38	Pass
STVE-1239	02/01/11	Cs-134	5.18 ± 0.19	5.50	3.85 - 7.15	Pass
STVE-1239	02/01/11	Cs-137	< 0.09	0.00	-	Pass
STVE-1239	02/01/11	Mn-54	6.91 ± 0.25	6.40	4.48 - 8.32	Pass
STVE-1239	02/01/11	Zn-65	3.10 ± 0.32	2.99	2.09 - 3.89	Pass
STSO-1240	02/01/11	Co-57	984.10 ± 4.10	927.00	649.00 - 1205.00	Pass
STSO-1240	02/01/11	Co-60	540.70 ± 3.00	482.00	337.00 - 627.00	Pass
STSO-1240	02/01/11	Cs-134	726.70 ± 5.92	680.00	476.00 - 884.00	Pass
STSO-1240	02/01/11	Cs-137	883.10 ± 4.70	758.00	531.00 - 985.00	Pass
STSO-1240	02/01/11	K-40	622.70 ± 16.70	540.00	378.00 - 702.00	Pass
STSO-1240	02/01/11	Mn-54	-0.30 ± 1.00	0.00	-	Pass
STSO-1240 ¹	02/01/11	Ni-63	384.00 ± 16.90	582.00	407.00 - 757.00	Fail
STSO-1240	02/01/11	U-233/4	166.60 ± 7.30	176.00	123.00 - 229.00	Pass
STSO-1240	02/01/11	U-238	172.00 ± 7.40	184.00	129.00 - 239.00	Pass
STSO-1240	02/01/11	Zn-65	1671.00 ± 13.10	1359.00	951.00 - 1767.00	Pass
STAP-1241	02/01/11	Am-241	0.00 ± 0.01	0.00	-0.10 - 0.10	Pass
STAP-1241	02/01/11	Co-57	3.48 ± 0.06	3.33	2.33 - 4.33	Pass
STAP-1241	02/01/11	Co-60	0.00 ± 0.02	0.00	-0.10 - 0.10	Pass
STAP-1241	02/01/11	Cs-134	3.44 ± 0.27	3.49	2.44 - 4.54	Pass
STAP-1241	02/01/11	Cs-137	2.46 ± 0.27	2.28	1.60 - 2.96	Pass

TABLE A-6. Department of Energy's Mixed Analyte Performance Evaluation Program (MAPEP)^a.

Lab Code ^c	Date	Analysis	Laboratory result	Concentration ^b		Acceptance
				Known Activity	Control Limits ^d	
STAP-1241	02/01/11	Gr. Alpha	0.39 ± 0.05	0.66	0.20 - 1.12	Pass
STAP-1241	02/01/11	Gr. Beta	1.54 ± 0.07	1.32	0.66 - 1.99	Pass
STAP-1241	02/01/11	Mn-54	2.90 ± 0.10	2.64	1.85 - 3.43	Pass
STAP-1241	02/01/11	Pu-238	0.07 ± 0.02	0.10	0.07 - 0.13	Pass
STAP-1241	02/01/11	Pu-239/40	0.06 ± 0.02	0.08	0.05 - 0.10	Pass
STAP-1241 ^g	02/01/11	Sr-90	1.89 ± 0.15	1.36	0.95 - 1.77	Fail
STAP-1241	02/01/11	U-233/4	0.13 ± 0.02	0.18	0.13 - 0.23	Pass
STAP-1241	02/01/11	U-238	0.14 ± 0.02	0.19	0.13 - 0.24	Pass
STAP-1241	02/01/11	Zn-65	3.80 ± 0.18	3.18	2.23 - 4.13	Pass
STW-1249	08/01/11	I-129	7.32 ± 0.30	9.50	6.70 - 12.40	Pass
STVE-1250	08/01/11	Co-57	0.01 ± 0.02	0.00	-	Pass
STVE-1250	08/01/11	Co-60	3.57 ± 0.13	3.38	2.37 - 4.39	Pass
STVE-1250	08/01/11	Cs-134	-0.02 ± 0.04	0.00	-0.10 - 0.10	Pass
STVE-1250	08/01/11	Cs-137	5.28 ± 0.20	4.71	3.30 - 6.12	Pass
STVE-1250	08/01/11	Mn-54	6.48 ± 0.22	5.71	4.00 - 7.42	Pass
STVE-1250	08/01/11	Zn-65	7.35 ± 0.34	6.39	4.47 - 8.31	Pass
STSO-1251	08/01/11	Co-57	1333.90 ± 4.20	1180.00	826.00 - 1534.00	Pass
STSO-1251	08/01/11	Co-60	701.30 ± 3.40	644.00	451.00 - 837.00	Pass
STSO-1251	08/01/11	Cs-134	0.71 ± 1.05	0.00	-	Pass
STSO-1251	08/01/11	Cs-137	1106.00 ± 5.60	979.00	685.00 - 1273.00	Pass
STSO-1251	08/01/11	K-40	749.20 ± 19.00	625.00	438.00 - 813.00	Pass
STSO-1251	08/01/11	Mn-54	984.30 ± 5.40	848.00	594.00 - 1102.00	Pass
STSO-1251	08/01/11	Ni-63	0.11 ± 1.21	0.00	-	Pass
STSO-1251	08/01/11	Pu-238	97.90 ± 7.40	93.60	65.50 - 121.70	Pass
STSO-1251	08/01/11	Pu-239/40	78.80 ± 6.40	77.40	54.20 - 100.60	Pass
STSO-1251 ⁿ	08/01/11	Sr-90	219.40 ± 16.70	320.00	224.00 - 416.00	Fail
STSO-1251 ⁱ	08/01/11	Tc-99	110.00 ± 8.00	182.00	127.00 - 237.00	Fail
STSO-1251	08/01/11	U-233/4	267.00 ± 10.20	263.00	184.00 - 342.00	Pass
STSO-1251	08/01/11	U-238	280.30 ± 10.40	274.00	192.00 - 356.00	Pass
STSO-1251	08/01/11	Zn-65	1639.90 ± 11.40	1560.00	1092.00 - 2028.00	Pass
STAP-1252	08/01/11	Co-57	5.06 ± 0.08	5.09	3.56 - 6.62	Pass
STAP-1252	08/01/11	Co-60	3.13 ± 0.09	3.20	2.24 - 4.16	Pass
STAP-1252	08/01/11	Cs-134	0.01 ± 0.03	0.00	-0.10 - 0.10	Pass
STAP-1252	08/01/11	Cs-137	2.61 ± 0.09	2.60	1.82 - 3.38	Pass
STAP-1252	08/01/11	Mn-54	0.01 ± 0.03	0.00	-0.10 - 0.10	Pass
STAP-1252	08/01/11	Pu-238	0.13 ± 0.02	0.12	0.08 - 0.15	Pass
STAP-1252	08/01/11	Pu-239/40	0.15 ± 0.02	0.14	0.10 - 0.18	Pass
STAP-1252	08/01/11	Sr-90	1.65 ± 0.16	1.67	1.17 - 2.17	Pass

TABLE A-6. Department of Energy's Mixed Analyte Performance Evaluation Program (MAPEP)^a.

Lab Code ^c	Date	Analysis	Laboratory result	Concentration ^b		Acceptance
				Known Activity	Control Limits ^d	
STAP-1252	08/01/11	U-233/4	0.17 ± 0.02	0.16	0.11 - 0.21	Pass
STAP-1252	08/01/11	U-238	0.17 ± 0.02	0.17	0.12 - 0.22	Pass
STAP-1252	08/01/11	Zn-65	4.46 ± 0.23	4.11	2.88 - 5.34	Pass
STW-1254	08/01/11	Co-57	37.20 ± 0.50	36.60	25.60 - 47.60	Pass
STW-1254	08/01/11	Co-60	28.80 ± 0.40	29.30	20.50 - 38.10	Pass
STW-1254	08/01/11	Cs-134	18.00 ± 0.60	19.10	13.40 - 24.80	Pass
STW-1254	08/01/11	Cs-137	0.06 ± 0.13	0.00	-	Pass
STW-1254	08/01/11	H-3	1039.90 ± 17.90	1014.00	710.00 - 1318.00	Pass
STW-1254	08/01/11	K-40	161.40 ± 4.10	156.00	109.00 - 203.00	Pass
STW-1254	08/01/11	Mn-54	25.70 ± 0.50	25.00	17.50 - 32.50	Pass
STW-1254	08/01/11	Ni-63	0.60 ± 2.00	0.00	-	Pass
STW-1254	08/01/11	Pu-238	0.04 ± 0.02	0.02	0.00 - 1.00	Pass
STW-1254	08/01/11	Pu-239/40	2.27 ± 0.14	2.40	1.68 - 3.12	Pass
STW-1254	08/01/11	Sr-90	15.60 ± 1.80	14.20	9.90 - 18.50	Pass
STW-1254	08/01/11	Tc-99	-0.30 ± 0.50	0.00	-	Pass
STW-1254	08/01/11	U-233/4	2.78 ± 0.20	2.78	1.95 - 3.61	Pass
STW-1254	08/01/11	U-238	2.86 ± 0.21	2.89	2.02 - 3.76	Pass
STW-1254	08/01/11	Zn-65	30.20 ± 0.90	28.50	20.00 - 37.10	Pass
STW-1255	08/01/11	Gr. Alpha	0.72 ± 0.12	0.87	0.26 - 1.47	Pass
STW-1255	08/01/11	Gr. Beta	4.71 ± 0.15	4.81	2.41 - 7.22	Pass

^a Results obtained by Environmental, Inc., Midwest Laboratory as a participant in the Department of Energy's Mixed Analyte Performance Evaluation Program, Idaho Operations office, Idaho Falls, Idaho

^b Results are reported in units of Bq/kg (soil), Bq/L (water) or Bq/total sample (filters, vegetation).

^c Laboratory codes as follows: STW (water), STAP (air filter), STSO (soil), STVE (vegetation).

^d MAPEP results are presented as the known values and expected laboratory precision (1 sigma, 1 determination) and control limits as defined by the MAPEP. A known value of "zero" indicates an analysis was included in the testing series as a "false positive". MAPEP does not provide control limits.

^e Result of a repeat analysis was still unacceptable. ERA crosschecks for Am-241 were acceptable, but biased low. Matrix spikes were prepared, (5.17 and 51.7 pCi/L), to verify method; results were acceptable, 4.4 and 47.5 pCi/L. Am-241 has been added to the internal spike and blank program for 2012.

^f An error in percent recovery was found, result of recalculation, 427.3 ± 18.8 Bq/kg dry.

^g No errors found in calculation or procedure, results of reanalysis; 1.73 Bq/filter.

^h The analyses were repeated through a strontium column; mean result of triplicate analyses, 304.2 Bq/kg.

ⁱ The lab does not currently analyze soil for Tc-99, but is evaluating the procedure. After consultation with Eichrom, the analysis was repeated using a matrix spike correction. Mean result of triplicate reanalyses; 183.3 Bq/kg.

TABLE A-7. Interlaboratory Comparison Crosscheck program, Environmental Resource Associates (ERA)^a.

Lab Code ^b	Date	Analysis	Concentration (pCi/L) ^b			Acceptance
			Laboratory Result ^c	ERA Result ^d	Control Limits	
STAP-1230	03/21/11	Am-241	46.0 ± 1.8	62.5	36.6 - 85.7	Pass
STAP-1230	03/21/11	Co-60	401.2 ± 12.1	390.0	302.0 - 487.0	Pass
STAP-1230	03/21/11	Cs-134	268.2 ± 24.8	279.0	182.0 - 345.0	Pass
STAP-1230	03/21/11	Cs-137	345.3 ± 24.9	312.0	234.0 - 410.0	Pass
STAP-1230	03/21/11	Mn-54	< 1.9	0.0	-	Pass
STAP-1230	03/21/11	Pu-238	76.1 ± 3.2	69.0	47.4 - 90.7	Pass
STAP-1230	03/21/11	Pu-239/40	70.50 ± 3.10	65.5	47.5 - 85	Pass
STAP-1230	03/21/11	Sr-90	208.40 ± 18.70	185.0	81.4 - 288	Pass
STAP-1230	03/21/11	U-233/4	56.10 ± 2.10	61.5	38.7 - 91	Pass
STAP-1230	03/21/11	U-238	58.90 ± 2.60	61.0	39.0 - 87	Pass
STAP-1230	03/21/11	Uranium	118.50 ± 5.52	125.0	63.9 - 199	Pass
STAP-1230	03/21/11	Zn-65	312.60 ± 23.40	279.0	193.0 - 386	Pass
STAP-1231	03/21/11	Gr. Alpha	88.40 ± 3.70	74.3	38.5 - 112	Pass
STAP-1231	03/21/11	Gr. Beta	85.10 ± 2.80	69.5	42.8 - 102	Pass
STSO-1232	03/21/11	Ac-228	1327.8 ± 97.5	1490.0	958.0 - 2100.0	Pass
STSO-1232	03/21/11	Am-241	662.8 ± 88.1	914.0	546.0 - 1170.0	Pass
STSO-1232	03/21/11	Bi-212	1396.2 ± 185.3	1400.0	368.0 - 2090.0	Pass
STSO-1232	03/21/11	Bi-214	841.1 ± 33.2	725.0	445.0 - 1040.0	Pass
STSO-1232	03/21/11	Co-60	2423.7 ± 27.1	2220.0	1620.0 - 2980.0	Pass
STSO-1232	03/21/11	Cs-134	2481.3 ± 42.2	2450.0	1580.0 - 2950.0	Pass
STSO-1232	03/21/11	Cs-137	2108.2 ± 30.2	1920.0	1470.0 - 2490.0	Pass
STSO-1232	03/21/11	K-40	11497.3 ± 276.6	11500.0	8320.0 - 15600.0	Pass
STSO-1232	03/21/11	Mn-54	< 17.4	0.0	-	Pass
STSO-1232	03/21/11	Pb-212	994.7 ± 30.0	1440.0	931.0 - 2030.0	Pass
STSO-1232	03/21/11	Pb-214	918.3 ± 42.6	805.0	482.0 - 1200.0	Pass
STSO-1232	03/21/11	Pu-238	1593.6 ± 156.7	1420.0	813.0 - 2000.0	Pass
STSO-1232	03/21/11	Pu-239/40	1428.9 ± 143.4	1400.0	956.0 - 1860.0	Pass
STSO-1232	03/21/11	Sr-90	8638.0 ± 442.8	7590.0	2740.0 - 12400.0	Pass
STSO-1232	03/21/11	Th-234	1350.1 ± 180.0	962.0	305.0 - 1830.0	Pass
STSO-1232	03/21/11	U-233/4	748.0 ± 94.4	972.0	616.0 - 1210.0	Pass
STSO-1232	03/21/11	U-238	909.0 ± 104.9	962.0	588.0 - 1220.0	Pass
STSO-1232	03/21/11	Uranium	1690.8 ± 104.9	1980.0	1130.0 - 2670.0	Pass
STSO-1232	03/21/11	Zn-65	2356.2 ± 57.1	1990.0	1580.0 - 2670.0	Pass

TABLE A-7. Interlaboratory Comparison Crosscheck program, Environmental Resource Associates (ERA)^a.

Lab Code ^b	Date	Analysis	Concentration (pCi/L) ^b		Control Limits	Acceptance
			Laboratory Result ^c	ERA Result ^d		
STVE-1233	03/21/11	Am-241	2377.5 ± 83.2	3200.0	1820.0 - 4400.0	Pass
STVE-1233	03/21/11	Cm-244	602.9 ± 38.4	812.0	400.0 - 1260.0	Pass
STVE-1233	03/21/11	Co-60	810.2 ± 32.4	733.0	496.0 - 1050.0	Pass
STVE-1233	03/21/11	Cs-134	849.4 ± 54.5	770.0	441.0 - 1070.0	Pass
STVE-1233	03/21/11	Cs-137	889.9 ± 36.3	829.0	608.0 - 1150.0	Pass
STVE-1233	03/21/11	K-40	28146.70 ± 698.80	25800.0	18500.0 - 36500	Pass
STVE-1233	03/21/11	Mn-54	< 19.3	0.0	-	Pass
STVE-1233	03/21/11	Pu-238	3068.10 ± 170.70	2990.0	1610.0 - 4380	Pass
STVE-1233	03/21/11	Pu-239/40	3180.00 ± 88.90	3100.0	1920.0 - 4230	Pass
STVE-1233	03/21/11	Sr-90	8549.20 ± 675.00	7890.0	4410.0 - 10500	Pass
STVE-1233	03/21/11	U-233/4	2418.60 ± 142.50	2610.0	1790.0 - 3460	Pass
STVE-1233	03/21/11	U-238	2417.00 ± 142.50	2590.0	1820.0 - 3270	Pass
STVE-1233	03/21/11	Uranium	4929.80 ± 142.50	5320.0	3660.0 - 6860	Pass
STVE-1233	03/21/11	Zn-65	962.40 ± 62.50	799.0	577.0 - 1090	Pass
STW-1234	03/21/11	Am-241	100.0 ± 6.4	135.0	92.5 - 182.0	Pass
STW-1234	03/21/11	Co-60	401.6 ± 7.2	411.0	358.0 - 486.0	Pass
STW-1234	03/21/11	Cs-134	222.7 ± 12.3	231.0	171.0 - 265.0	Pass
STW-1234	03/21/11	Cs-137	410.3 ± 9.5	417.0	354.0 - 500.0	Pass
STW-1234	03/21/11	Mn-54	< 3.0	0.0	-	Pass
STW-1234	03/21/11	Pu-238	130.9 ± 5.5	131.0	99.1 - 162.0	Pass
STW-1234	03/21/11	Pu-239/40	113.0 ± 5.0	119.0	92.1 - 147.0	Pass
STW-1234	03/21/11	Sr-90	739.6 ± 13.0	773.0	491.0 - 1030.0	Pass
STW-1234	03/21/11	U-233/4	83.4 ± 3.8	94.3	71.1 - 122.0	Pass
STW-1234	03/21/11	U-238	85.5 ± 3.9	93.5	71.4 - 116.0	Pass
STW-1234	03/21/11	Uranium	172.0 ± 8.5	192.0	138.0 - 256.0	Pass
STW-1234	03/21/11	Zn-65	114.5 ± 10.8	111.0	94.1 - 138.0	Pass
STW-1235	03/21/11	Gr. Alpha	97.6 ± 2.9	112.0	49.7 - 166.0	Pass
STW-1235	03/21/11	Gr. Beta	99.6 ± 2.0	99.8	58.4 - 146.0	Pass
STW-1236	03/21/11	H-3	16307.0 ± 377.0	15200.0	9900.0 - 22500.0	Pass

^a Results obtained by Environmental, Inc., Midwest Laboratory as a participant in the crosscheck program for proficiency testing administered by Environmental Resources Associates, serving as a replacement for studies conducted previously by the Environmental Measurements Laboratory Quality Assessment Program (EML).

^b Laboratory codes as follows: STW (water), STAP (air filter), STSO (soil), STVE (vegetation). Results are reported in units of pCi/L, except for air filters (pCi/Filter), vegetation and soil (pCi/kg).

^c Unless otherwise indicated, the laboratory result is given as the mean ± standard deviation for three determinations.

^d Results are presented as the known values, expected laboratory precision (1 sigma, 1 determination) and control limits as provided by ERA. A known value of "zero" indicates an analysis was included in the testing series as a "false positive". Control limits are not provided.

APPENDIX B

DATA REPORTING CONVENTIONS

Data Reporting Conventions

1.0. All activities, except gross alpha and gross beta, are decay corrected to collection time or the end of the collection period.

2.0. Single Measurements

Each single measurement is reported as follows: $x \pm s$
where: x = value of the measurement;
 s = 2σ counting uncertainty (corresponding to the 95% confidence level).

In cases where the activity is less than the lower limit of detection L , it is reported as: $< L$, where L = the lower limit of detection based on 4.66σ uncertainty for a background sample.

3.0. Duplicate analyses

If duplicate analyses are reported, the convention is as follows. :

- 3.1 Individual results: For two analysis results; $x_1 \pm s_1$ and $x_2 \pm s_2$
Reported result: $x \pm s$; where $x = (1/2)(x_1 + x_2)$ and $s = (1/2) \sqrt{s_1^2 + s_2^2}$
- 3.2. Individual results: $< L_1, < L_2$ Reported result: $< L$, where L = lower of L_1 and L_2
- 3.3. Individual results: $x \pm s, < L$ Reported result: $x \pm s$ if $x \geq L$; $< L$ otherwise.

4.0. Computation of Averages and Standard Deviations

4.1 Averages and standard deviations listed in the tables are computed from all of the individual measurements over the period averaged; for example, an annual standard deviation would not be the average of quarterly standard deviations. The average \bar{x} and standard deviation "s" of a set of n numbers x_1, x_2, \dots, x_n are defined as follows:

$$\bar{x} = \frac{1}{n} \sum x \qquad s = \sqrt{\frac{\sum (x - \bar{x})^2}{n-1}}$$

- 4.2 Values below the highest lower limit of detection are not included in the average.
- 4.3 If all values in the averaging group are less than the highest LLD, the highest LLD is reported.
- 4.4 If all but one of the values are less than the highest LLD, the single value x and associated two sigma error is reported.
- 4.5 In rounding off, the following rules are followed:
- 4.5.1. If the number following those to be retained is less than 5, the number is dropped, and the retained numbers are kept unchanged. As an example, 11.443 is rounded off to 11.44.
- 4.5.2. If the number following those to be retained is equal to or greater than 5, the number is dropped and the last retained number is raised by 1. As an example, 11.445 is rounded off to 11.45.

APPENDIX C

Maximum Permissible Concentrations
of Radioactivity in Air and Water
Above Background in Unrestricted Areas

Table C-1. Maximum permissible concentrations of radioactivity in air and water above natural background in unrestricted areas^a.

Air (pCi/m ³)		Water (pCi/L)	
Gross alpha	1×10^{-3}	Strontium-89	8,000
Gross beta	1	Strontium-90	500
Iodine-131 ^b	2.8×10^{-1}	Cesium-137	1,000
		Barium-140	8,000
		Iodine-131	1,000
		Potassium-40 ^c	4,000
		Gross alpha	2
		Gross beta	10
		Tritium	1×10^6

^a Taken from Table 2 of Appendix B to Code of Federal Regulations Title 10, Part 20, and appropriate footnotes. Concentrations may be averaged over a period not greater than one year.

^b Value adjusted by a factor of 700 to reduce the dose resulting from the air-grass-cow-milk-child pathway.

^c A natural radionuclide.

APPENDIX D

Sampling Location Maps

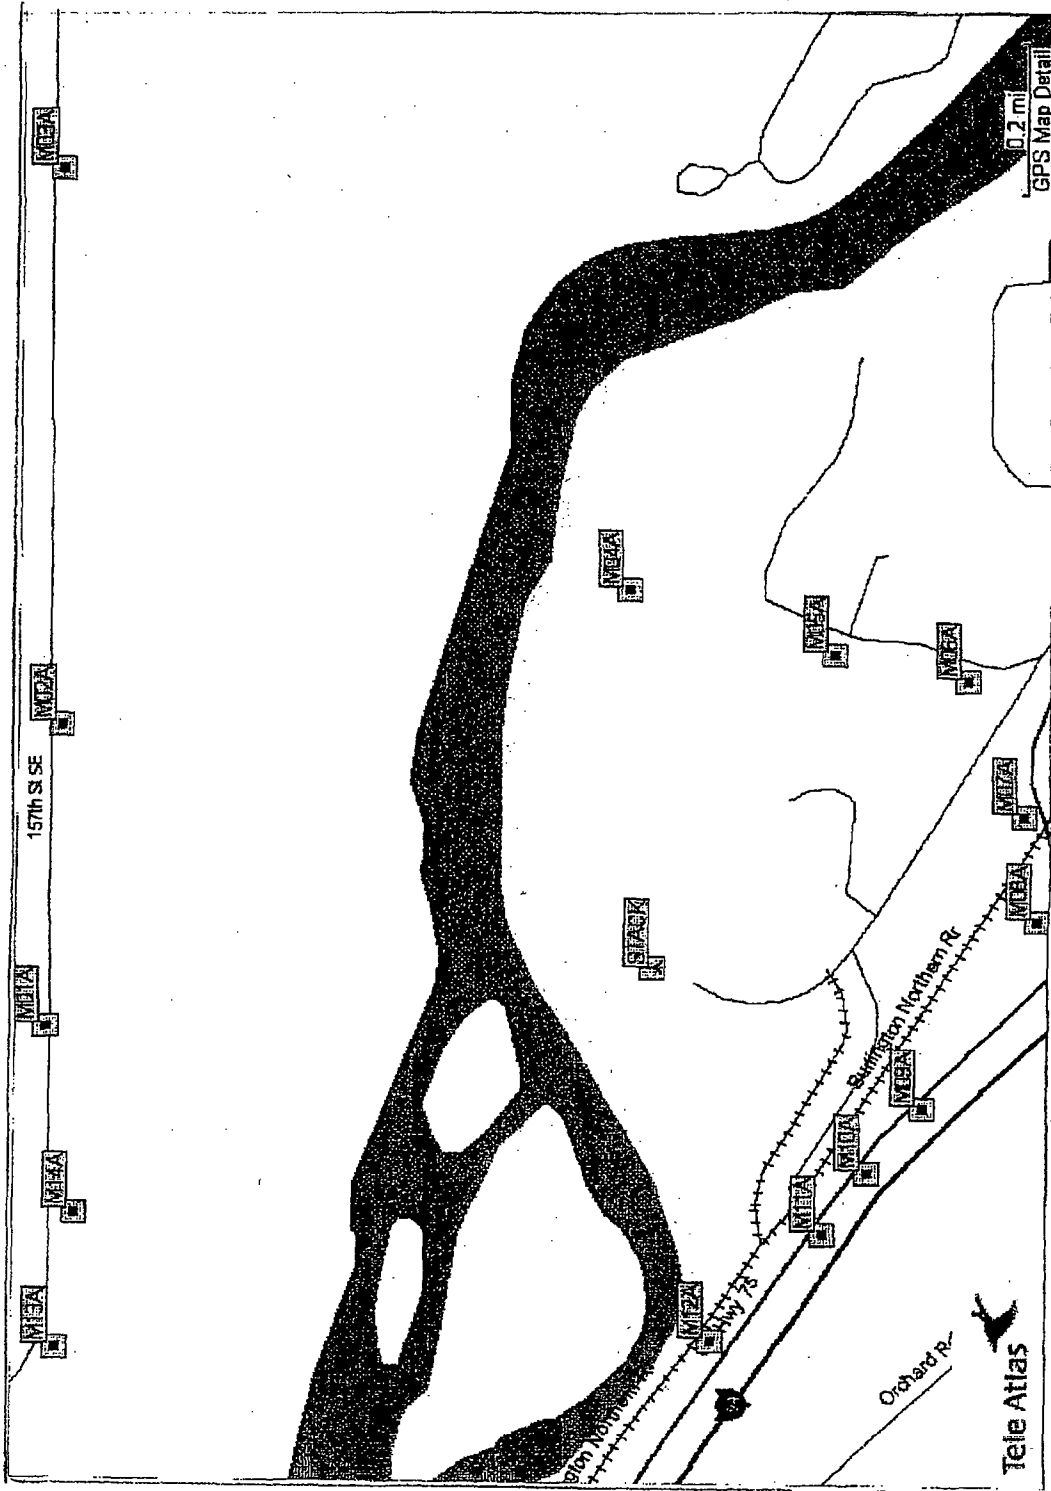


Figure D-1, Sample Collection and Analysis Program: TLD locations, Inner Ring. (Table 5.2)

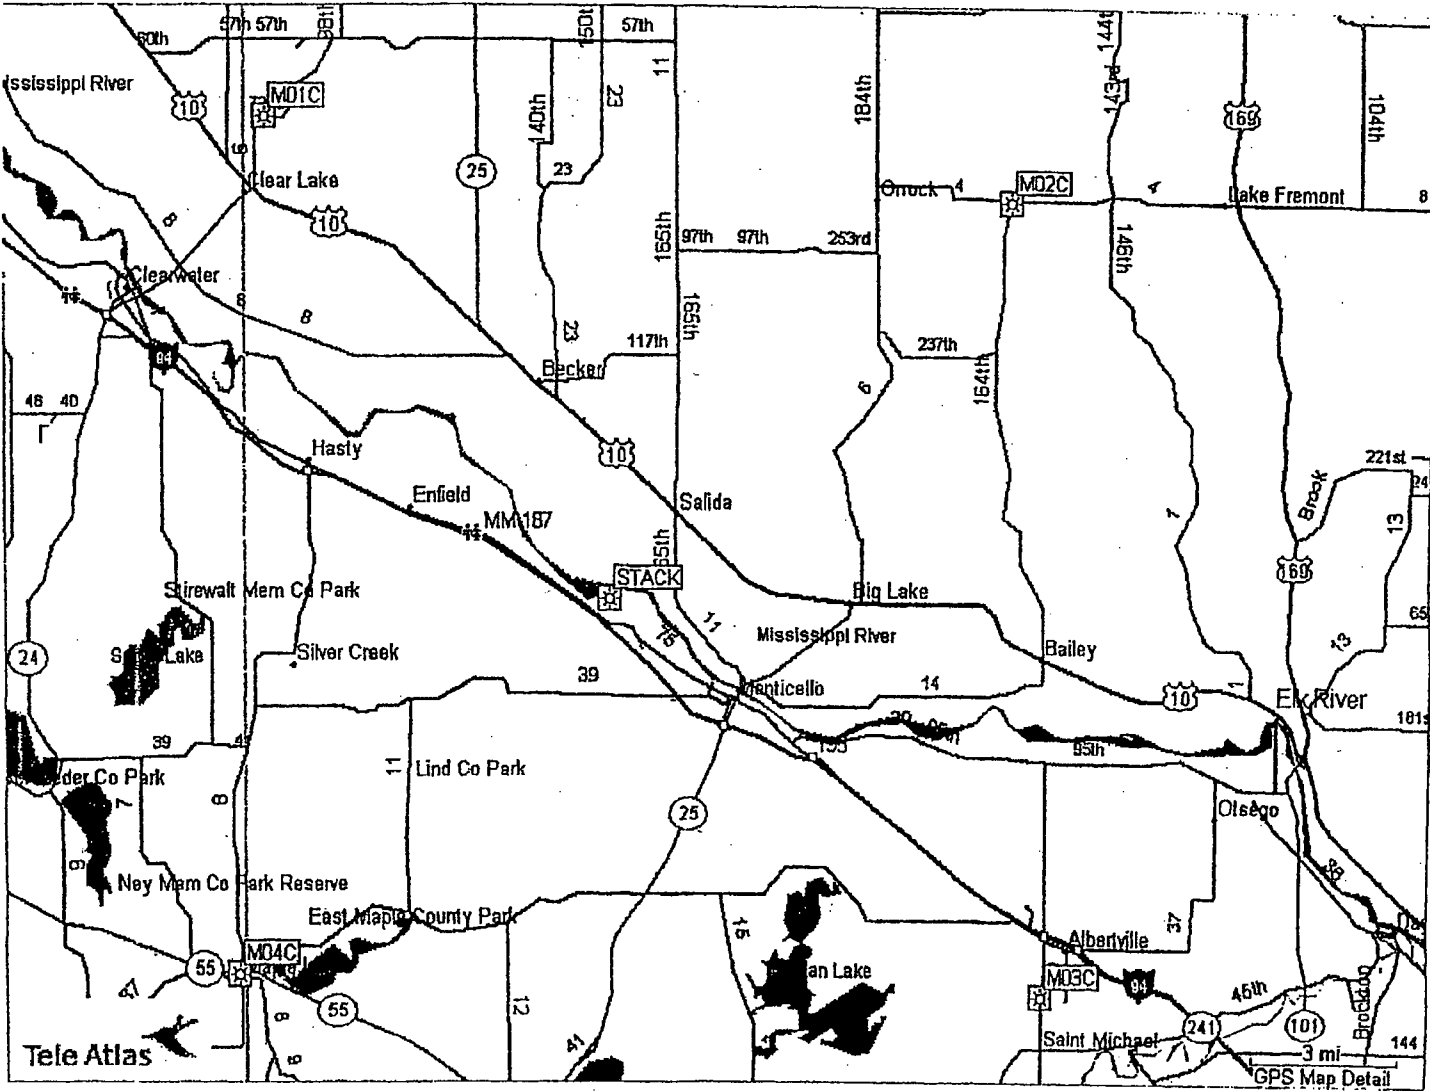


Figure D-3, Sample Collection and Analysis Program: TLD locations, Controls. (Table 5.2)

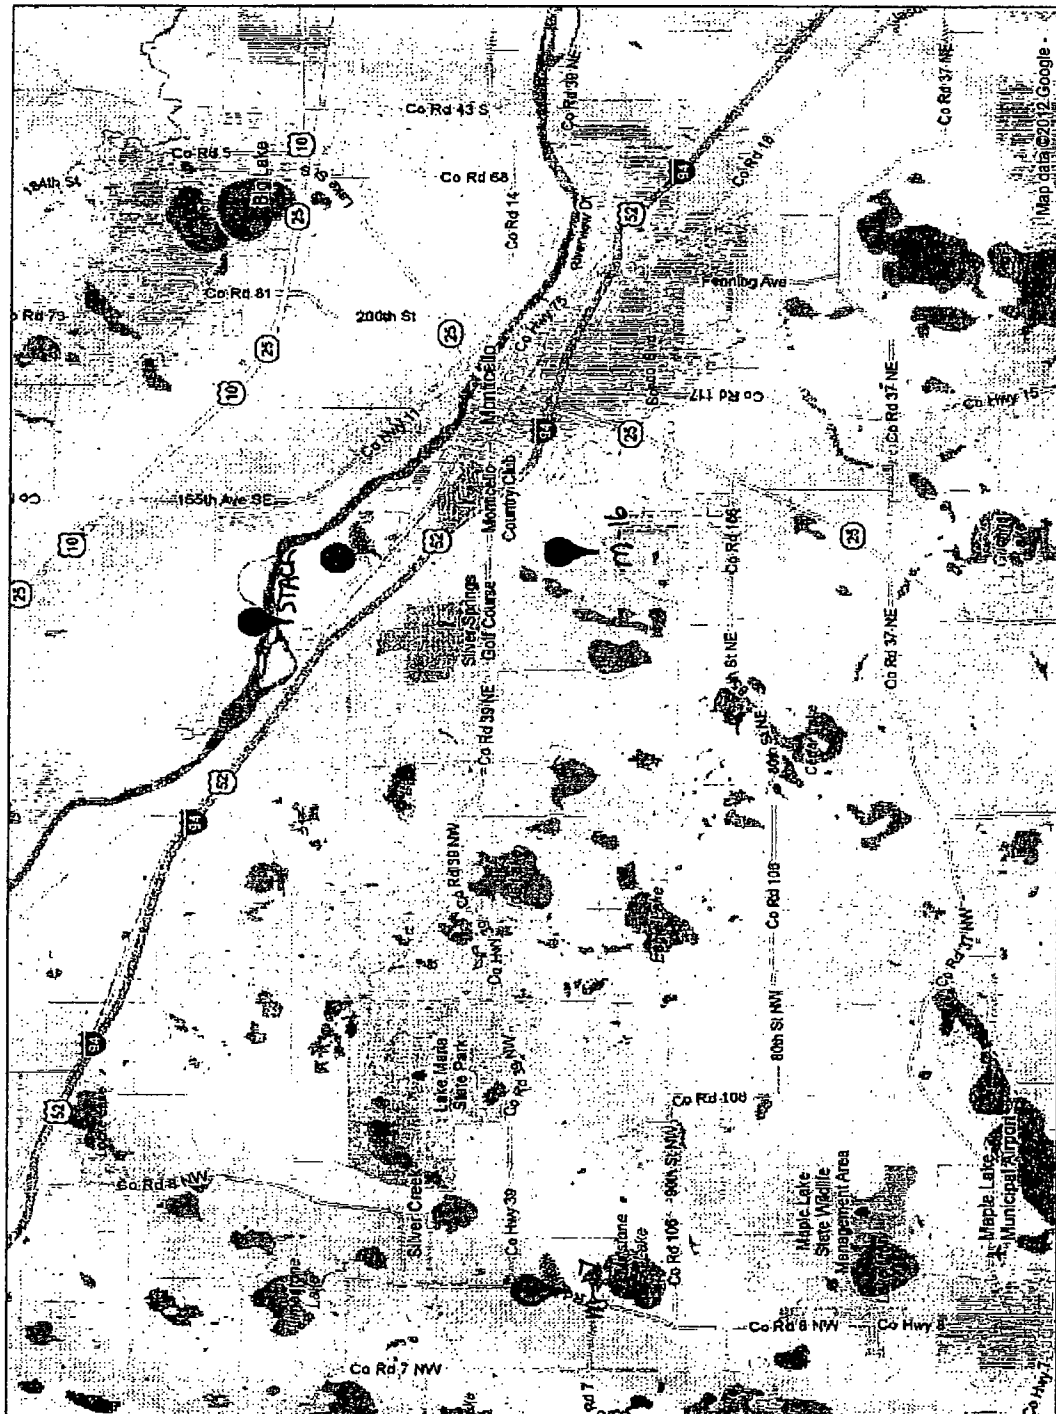


Figure D-4, Sample Collection and Analysis Program: Radiological Environmental Monitoring Program, Milk Sampling locations. (Table 5.2)

APPENDIX E

Ground Water Monitoring Well Samples

1.0 INTRODUCTION

This appendix to the Radiological Environmental Monitoring Program Annual Report to the United States Nuclear Regulatory Commission summarizes and interprets results of the Ground Water Monitoring Program samples taken at the Monticello Nuclear Plant, Monticello, Minnesota, during the period January – December 2011. This sampling program was established in October of 2006 following the industry initiative on ground water monitoring.

Complete data tables for each period and sampling location, are provided in a reference document, (Environmental, Inc., Midwest Laboratory, "Complete Analyses Data Tables, January – December, 2011") available at the Monticello Nuclear Generating Plant, Chemistry and Radiation Protection Department.

2.0 SUMMARY

The Ground Water Sampling Program was established following industry events where tritium was discovered in ground water surrounding commercial nuclear facilities. This program is described and the results for 2011 are summarized and discussed.

Program findings for 2011 detected low levels of tritium in monitoring wells located on the plant property at or near the expected natural background levels, with the exception of Monitoring Wells MW-9A and MW-10. The 2011 sample results (excluding MW-9A and MW-10) all measured below the required limit of 500 pCi/L. Storm water runoff samples ranged from 772 pCi/L to below 500 pCi/L. The measurements for 2011 are below the Environmental Protection Agency's drinking water standard of 20,000 pCi/L and present no harm to members of the public.

None of the samples monitored for gamma-emitting isotopes showed activity greater than the LLD.

A summation of the analytical data for both ground water monitoring wells and storm water runoff samples is provided in Table E-3.

3.0 Ground Water Sampling Program

3.1 Program Design and Data Interpretation

The purpose of this sampling program is to assess the impact of any tritium leaching into the environment (ground water system) from MNGP. For this purpose, water samples are collected and analyzed for tritium content.

3.2 Program Description

The sampling and analysis schedule for the Ground Water Monitoring Program is summarized in Table E-1 and briefly reviewed below. Table E-2 defines the additional sample locations and codes for the Ground Water Sampling Program.

Sampling from the groundwater monitoring wells was conducted monthly at twelve locations and quarterly for five locations.

3.3 Program Execution

The Ground Water Monitoring Program was executed as described in the preceding section. Monitoring Well M-14 was installed in the fall of 2010, but only one sample had been collected due to inaccessibility of the well. The well was sampled monthly in 2011.

3.4 Program Modifications

There were no changes to the program for 2011.

3.5 Results and Discussions

Results obtained show tritium in ground water samples at or near expected natural background levels, with the exception of monitoring wells, MW-9A and MW-10.

Excluding data for wells MW-9A and MW-10, the 2011 sample results are similar or slightly lower than averages seen in 2010 and within the range of expected background tritium levels in groundwater, due to tritium concentrations measured in precipitation. Sampling points in North America have shown tritium concentrations in precipitation ranging from 5 pCi/L to 157 pCi/L (Environmental Isotope Data No. 10; World Survey of Isotope Concentration in Precipitation (1988-1991)).

The tritium activity detected at sites MW-9A and MW-10 ranged from a high of 2317 pCi/L to < 500 pCi/L. The levels were significantly lower than measurements taken in 2010. Previous investigations concluded that the higher tritium activity was due to a 1981 spill from the Condensate Storage Tanks, that had infiltrated the surface and migrated towards MW-9.

None of the groundwater samples analyzed for gamma-emitting isotopes showed activity greater than LLD.

Table E-1. Sample Collection and Analysis Program, Ground Water.

Medium	Number	Sample Codes	Collection type	Analysis Type
Ground Water Quarterly	25	MW-4, MW-5, MW-6, MW-7, MW-8	Grab	H-3, Gamma
Ground Water Monthly	142	MW-1, MW-2, MW-3, MW-9A, MW-9B, MW-10, MW-11, MW-12A, MW-12B, MW-13A, MW-13B, MW-14	Grab	H-3

Table E-2. Sampling locations for Ground Water Monitoring Wells.

Sample Type	Vendor Code	Well Number	Distance from Stack (miles)	Compass Heading from Stack	Sector
Ground Water	M-33	MW-1	0.11	299	WNW
Ground Water	M-34	MW-2	0.14	301	WNW
Ground Water	M-35	MW-3	0.15	305	NW
Ground Water	M-36	MW-4	0.1	25	NNE
Ground Water	M-37	MW-5	0.1	253	WSW
Ground Water	M-38	MW-6	229 Feet	228	SW
Ground Water	M-39	MW-7	0.2	66	ENE
Ground Water	M-40	MW-8	0.3	150	SSE
Ground Water	M-44	MW-9A	0.1	310	NW
Ground Water	M-51	MW-9B	0.1	310	NW
Ground Water	M-45	MW-10	0.1	292	WNW
Ground Water	M-46	MW-11	0.1	283	WNW
Ground Water	M-47	MW-12A	0.1	330	NW
Ground Water	M-48	MW-12B	0.1	326	NW
Ground Water	M-49	MW-13A	0.12	316	NW
Ground Water	M-50	MW-13B	0.12	316	NW
Ground Water	M-52	MW-14	0.17	306	NW

Table E-3. Ground Water Monitoring Program Summary.

Name of Facility Monticello Nuclear Generating Plant Docket No. 50-263
 Location of Facility Wright, Minnesota Reporting Period January-December, 2011
 (County, State)

Sample Type (Units)	Type and Number of Analyses ^a	LLD ^b	Indicator Locations Mean (F) ^c Range ^c	Location with Highest Annual Mean		Control Locations Mean (F) ^c Range ^c	Number Non-Routine Results ^e
				Location ^d	Mean (F) ^c Range ^c		
Groundwater Monitoring Wells (pCi/L)	H-3 166	500	819 (13/166) (540-2317)	MW-9A, Onsite, 0.1 mi,@ 310°/NW	1445 (3/12) (820-2317)	none	13
	GS 142						
	Mn-54 10	< LLD	-		-	none	0
	Fe-59 30	< LLD	-		-	none	0
	Co-58 10	< LLD	-		-	none	0
	Co-60 10	< LLD	-		-	none	0
	Zn-65 30	< LLD	-		-	none	0
	Zr-Nb-95 15	< LLD	-		-	none	0
	Cs-134 10	< LLD	-		-	none	0
	Cs-137 10	< LLD	-		-	none	0
Ba-La-140 15	< LLD	-	-	none	0		
Ce-144 56	< LLD	-	-	none	0		
Stormwater Runoff (pCi/L)	H-3 7	500	679 (2/7) (585-772)	Sewer Lift Station On-site	679 (2/7) (585-772)	none	2
	GS 3						
	Mn-54 10	< LLD	-		-	none	0
	Fe-59 30	< LLD	-		-	none	0
	Co-58 10	< LLD	-		-	none	0
	Co-60 10	< LLD	-		-	none	0
	Zn-65 30	< LLD	-		-	none	0
	Zr-Nb-95 15	< LLD	-		-	none	0
	I-131 30	< LLD	-		-	none	0
	Cs-134 10	< LLD	-		-	none	0
Cs-137 10	< LLD	-	-	none	0		
Ba-La-140 15	< LLD	-	-	none	0		
Ce-144 45	< LLD	-	-	none	0		

^a GB = gross beta, GS = gamma scan.

^b LLD = nominal lower limit of detection based on a 4.66 sigma counting error for background sample.

^c Mean and range are based on detectable measurements only. Fraction of detectable measurements at specified locations is indicated in parentheses (F).

^d Locations are specified: (1) by name, and/or station code and (2) by distance (miles) and direction relative to reactor site.

^e Non-routine results are those which exceed ten times the control station value. If no control station value is available, the result is considered non-routine if it exceeds ten times the typical preoperational value for the medium or location.

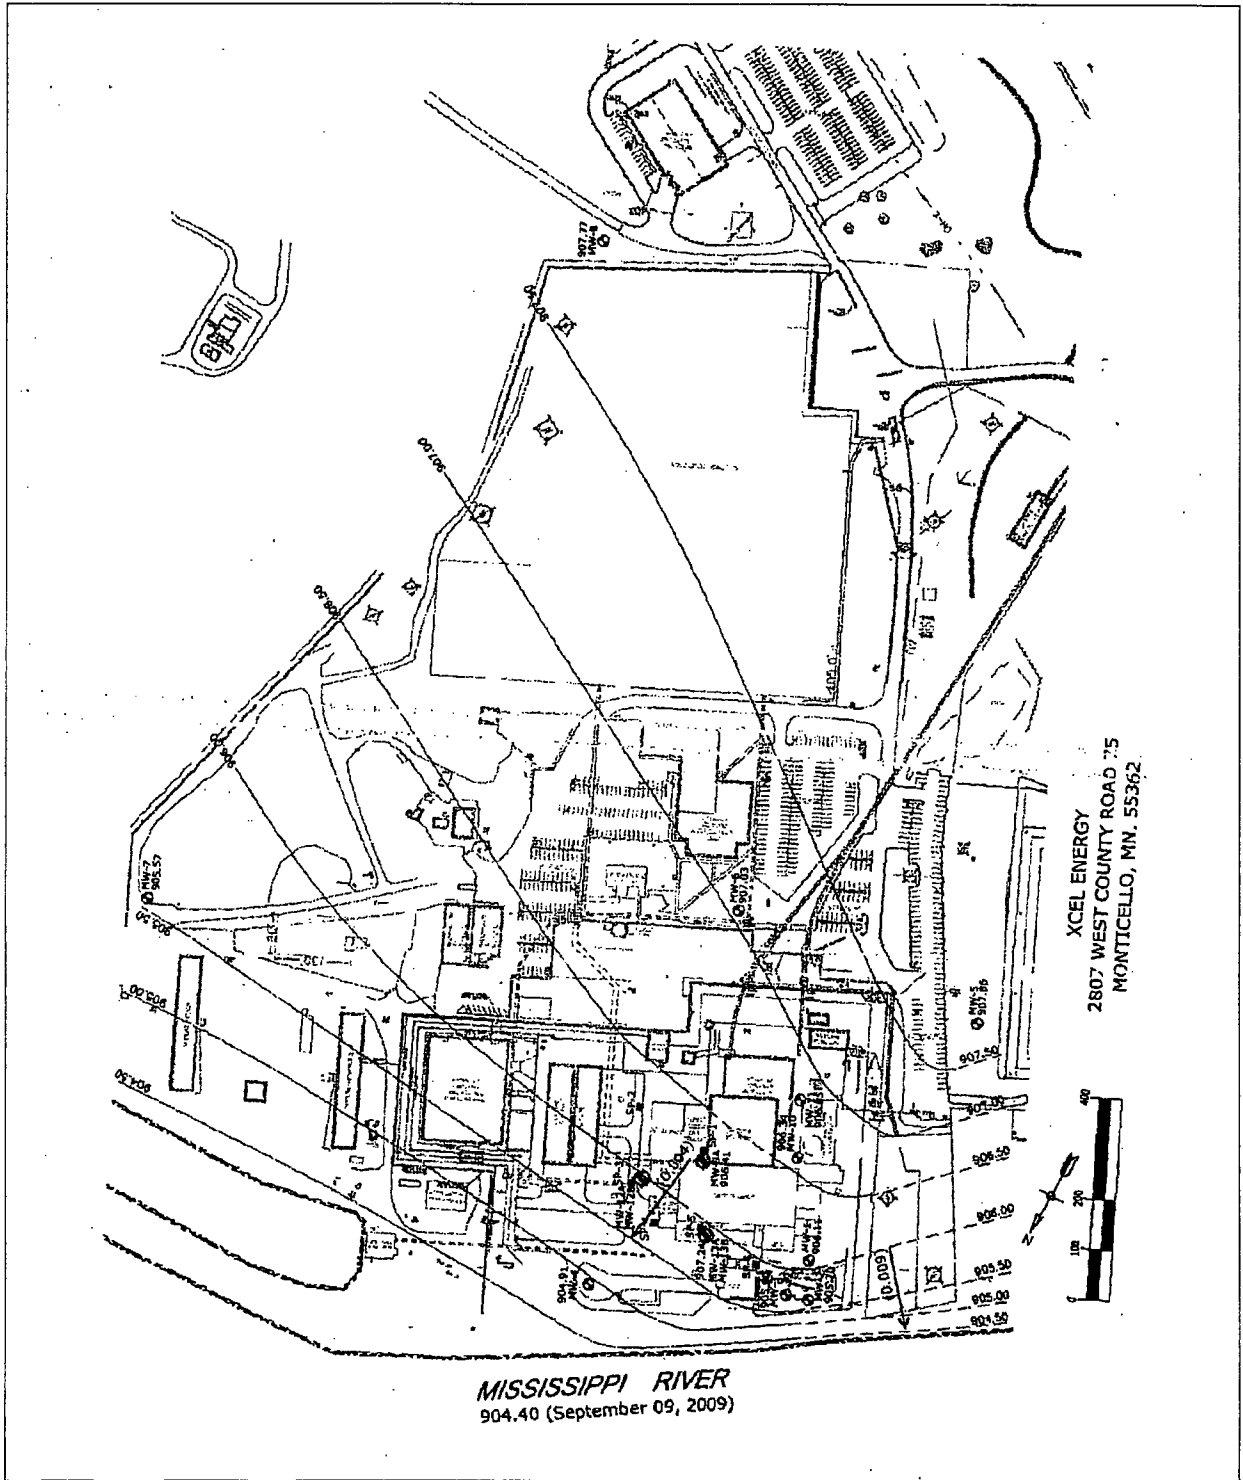


Figure E-1. Sample collection and analysis program: Ground water, On-site monitoring well locations.



SHIPPING DOCUMENT

NORTHERN STATES POWER -MN
Xcel Energy
 2807 County Rd 75 Monticello
 MN 55362

Date: 5-10-12

Shipping Document
 Tracking Number:

Ship To:
USNRC
 11555 Rockville Pike
 Rockville, MD 20852-2738

Attention Of: Document Control Desk

SHIPPING BY	SHIPMENT PACKAGING Pallet, Box, Etc.	SHIPMENT PO NUMBER:	RMA NO.:
Fed Ex		ORIGINAL PO NUMBER:	BUYER:
Town Run			
Motor Freight		FREIGHT TRACKING NO.	JDE NUMBER:
Vendor			
UPS		Reason for shipment: Overnight Shipment to USNRC	
Other			

Item No.	Qty	Unit	Description	Catalog ID / Q
1	1	Document	2011 Annual Radiological Environmental Operating Report	

Shipment Requester DeNae Sievers – Please ensure that a tracking number is communicated to me.	SWIP Making Shipment
--	-----------------------------